


Test Equipment
Depot
1-800-517-8431

5 Commonwealth Ave
Woburn, MA 01801
Phone 781-665-1400
Toll Free 1-800-517-8431

Visit us at www.TestEquipmentDepot.com

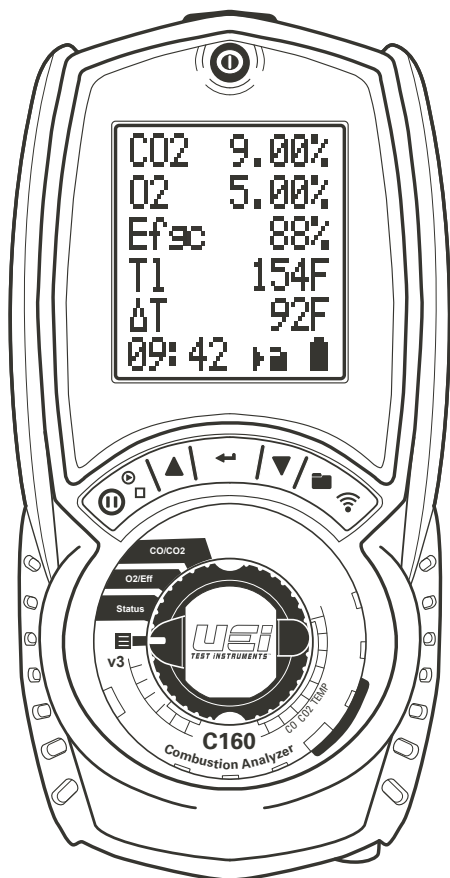

BACKED BY

Uei

SERVICE+

6


YEAR
WARRANTY

24


HR
SERVICE

FREE
SHIPPING

C160 OVERVIEW

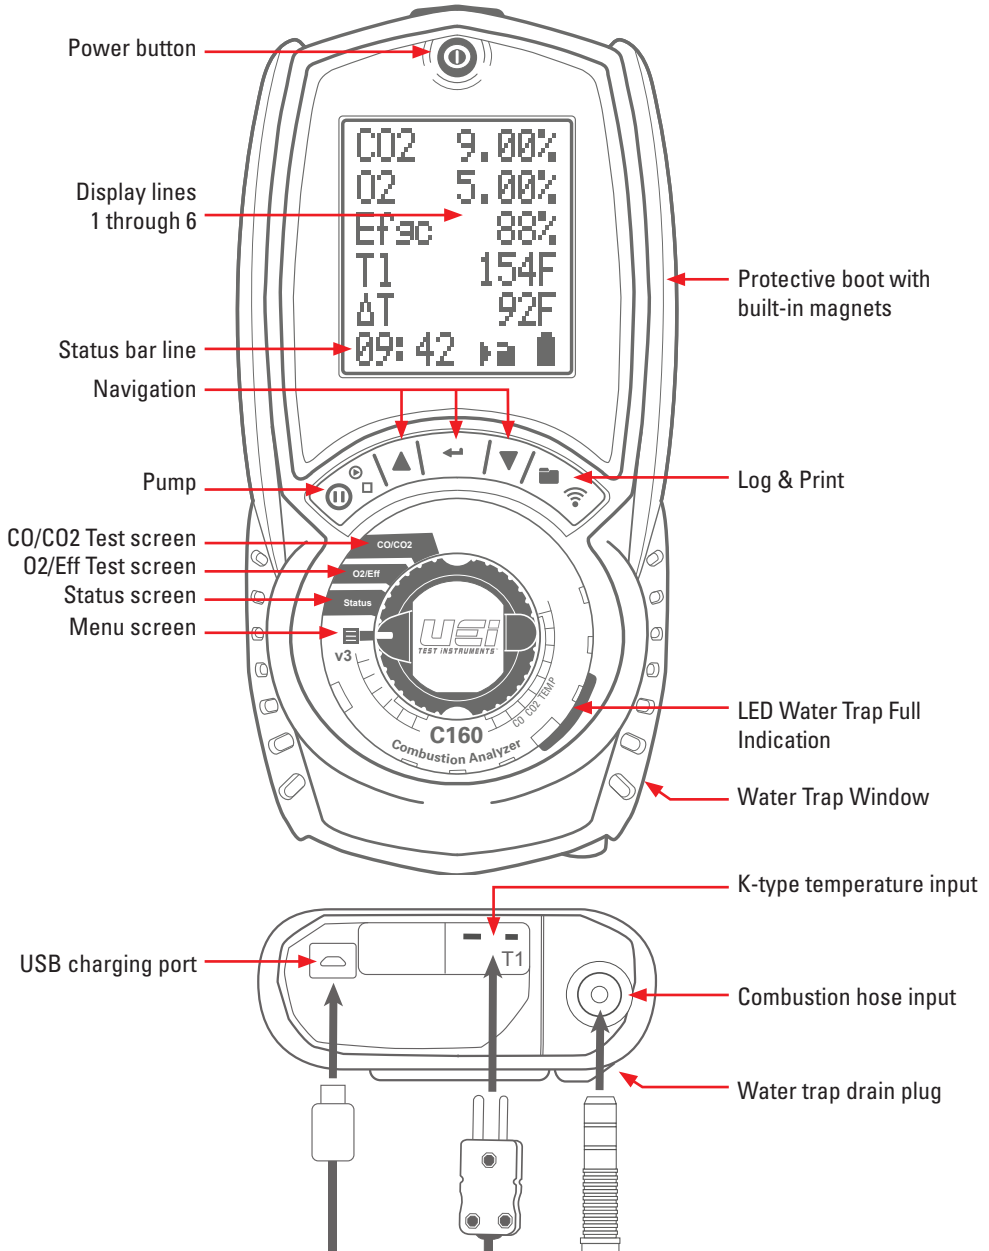

MENU SCREEN - C160 START UP


Press  "Power" Button for 2 seconds. The analyzer will perform a 60 second purge. This should be done in fresh air.

Rotate Selector Dial to **MENU** to set up or customize your settings.

Selected parameter are centered, highlighted with arrow icons on either side.


Use  and  buttons to scroll menu options,

Press  to select and edit a parameter.

Press  and  buttons to change contents of a field.

Press  button to scroll fields.

Press  to enter content and move to next field.

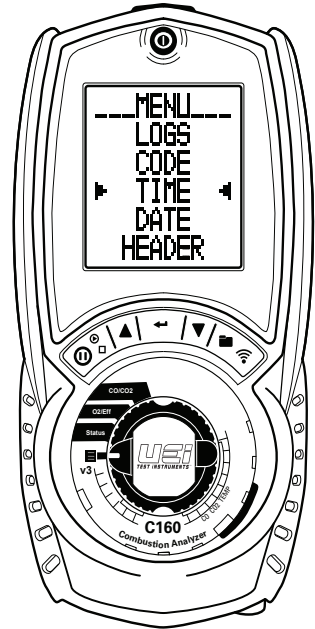

STATUS SCREEN

Rotate Selector Dial to **STATUS** to view parameters.

Selected Fuel

Ti = Ambient Temperature

CAL = Days remaining until calibration

Press  and  buttons to scroll Status Bar options.

Time, Pump Status, Battery Status

Fuel Type

Date


Change Fuel Type in STATUS SCREEN

Press  and  buttons to the currently selected fuel.

Press and Hold  button until arrows indicate fuel edit mode is activated.

The  and  to scroll fuel types.


Press  to select desired fuel.

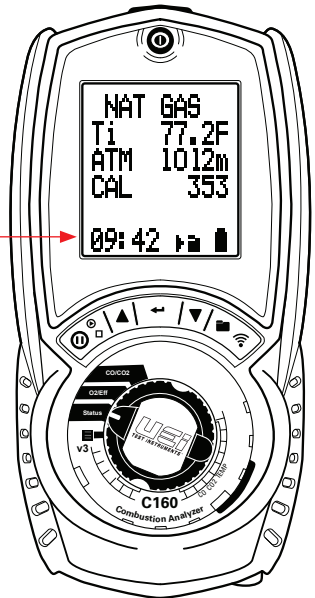


BEFORE TESTING

CHECKLIST

- Clean particle filter
- Water trap and probe line are free of water
- All hose and thermocouple connections are properly secured
- Water trap is fitted correctly
- Power on and zero
- Flue gas probe is sampling ambient FRESH air




Remove the rubber boot and red drain plug. Allow the water to drain out. Re-insert the rubber plug and replace boot cover.




Remove protective rubber boot. Remove water trap from analyzer. Remove particle filter from spigot and replace with new one. Reattach trap and boot.


COMBUSTION ANALYSIS



Insert flue probe into combustion input. Insert K-type temperature probe into input T1.




Insert flue probe into stack. Adjust cone so the probe tip is approximately at the center of the stack.




Rotate rotary dial to O2/Eff for O2/Eff Test Screen parameters.


NOTE: If there is no hole, check with service and installation instructions of appliance for best testing method or check with your local authority on best practice



O2/Eff displays O2 (%), Gross Efficiency, Flue Temperature.




Rotate rotary dial to CO/CO2 for CO/CO2 Test Screen parameters.




CO/CO2 displays CO (ppm), Losses calculated, Excess Air %, Make any adjustments needed for proper combustion and wait for changes in readings (Repeat necessary).


CHANGE FUEL TYPE



Rotate rotary dial to O2/Eff or CO/CO2 setting.




Press ▼ button until the Fuel Type displays on the Status Bar.
Press and Hold ◀ until two arrow icons display.

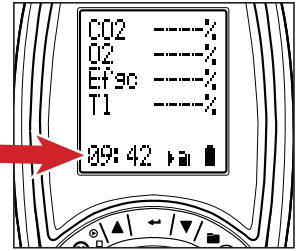


Press ▲ and ▼ buttons to scroll fuel selections.
Press ◀ to select fuel.


PRINTING & LOGGING



To Print: Align printer (sold separately) above Analyzer.




During testing, Press to start printing.
Press again to abort.

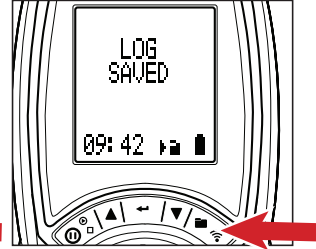


To Log: During testing, Press and Hold to log a report.
To view these Logs, see **View Saved Logs** section.


VIEW SAVED LOGS




Rotate the dial to MENU.
Press button until the LOGS is selected between two arrow icons. Press to select.




Screen displays all saved LOGS.
With VIEW selected in the Status Bar, Press to select.




Press and buttons to scroll Test Report categories.
Press to select a category.



Line 1 displays the LOG number on screen.
To view another LOG, Press and buttons to NEXT.
Press to advance to next log.
Repeat until you reach desired LOG.




To print the LOG, Press and buttons until PRINT is selected between two arrow icons. Press to select to start printing.



To EXIT, Press and buttons until EXIT is selected between two arrow icons. Press to EXIT screen.
Repeat until return to MENU screen.

POST TESTING



Remove the probe from the flue and allow analyzer to purge with fresh air until readings return to zero. O₂ to 20.9%, CO to Zero
CAUTION: probe tip will be HOT.

POWERING OFF


When you power off the C160, there is a 10 second purge.



Make sure you do not exceed the analyzer's operating specifications.

- Do not exceed the flue probes maximum temperature (1112°F, dependent on flue probe used)
- Do not exceed the analyzer's internal temperature range 112°F (50°C)
- Do not put the analyzer on a hot surface
- Do not exceed the water trap's level
- Do not let the particle filter become dirty and blocked

BATTERIES



The analyzer is fitted with 3 (AA) size rechargeable batteries. Observe correct polarity when replacing.

Always check operation immediately after battery replacement.

Do not leave batteries in unit for extended periods of non-use.



Do not recharge with Alkaline batteries fitted. Alkaline batteries are not rechargeable. Attempting to recharge alkaline batteries may result in product damage and create a fire risk.

Time and Date will need to be reset after changing batteries.

Always dispose batteries using approved disposal methods that protect the environment.

WARRANTY

The C160 combustion analyzer is warranted for one year including sensors. If within the warranty period your instrument should become inoperative from such defects, the unit will be repaired or replaced at UEi's option. This warranty covers normal use and does not cover damage which occurs in shipment or failure which results from alteration, tampering, accident, misuse, abuse, neglect or improper maintenance (calibration). Batteries and consequential damage resulting from failed batteries are not covered by warranty. Any implied warranties, including but not limited to implied warranties of merchantability and fitness for a particular purpose, are limited to the express warranty. UEi shall not be liable for loss of use of the instrument or other incidental or consequential damages, expenses, or economic loss, or for any claim or claims for such damage, expenses or economic loss. A purchase receipt or other proof of original purchase date will be required before warranty repairs will be rendered. Instruments out of warranty will be repaired (when repairable) for a service charge. Warranty only covers hardware and does not extend to software applications. Contact UEi for specific warranty and service information.

This warranty gives you specific legal rights. You may also have other rights which vary from state to state.

ANNUAL RECERTIFICATION SERVICES



Complete care for your C160 series combustion analyzer.

BACKED BY



When you:

***Request Recertification or Service Online
Within 1 Year of Purchase or Service***

6
YEAR
WARRANTY

UEi will:

6-Year Warranty: All UEi combustion analyzers have a standard 1-year warranty. Each recertification includes a 30-point inspection and extends the warranty for 1 more year for up to 6 years from the date of warranty.



24-hour Service: Analyzers received for standard recertification and service through UEi Service+ are shipped back on the next business day.



Free Shipping: UEi Service+ offers free shipping both to and from our service center. When customers book their recertification, they receive a prepaid UPS Ground shipping label.

Register Online

Registering you analyzer online is quick and easy. Just log in or setup an account, it only takes a couple of minutes. Once logged in you can register you analyzer by providing some product information and uploading a proof-of-purchase.

When it's time to request recertification, just log into your account, select the analyzer, select the service and place your order.

Test Equipment Depot - 800.517.8431 - 5 Commonwealth Ave, MA 01801

TestEquipmentDepot.com