HIOKI

SERI

DIGITAL MULTIMETER DT4200 Series



5 Commonwealth Ave Woburn, MA 01801 Phone 781-665-1400 Toll Free 1-800-517-8431

at www.TestEquipmentDepot.com



DT4261



Newly released "DT4261" for wireless communication and DC high voltage measurement!

DT4261 Bluetooth[®] wireless technology support for recording and managing measurement data



Bluetooth[®] communication with Z3210 attached to DT4261 Bluetooth[®]

Install the Wireless Adapter Z3210 to the DT4261 to enable Bluetooth[®] communications. With the Z3210, you can transfer data directly to an Excel[®] file or pair the instrument with GENNECT Cross.



Attach to enable Bluetooth® wireless technology









Manage measurement data using GENNECT Cross

Pair the DT4261 built in with Bluetooth[®] wireless technology with the free GENNECT Cross mobile app to further data management, processing and report exporting on your mobile device.



GENNECT



Transfer data to a tablet wirelessly



Take a picture of the test location and map measured values on it

			Ø
			al 📑 141
<home 14:09</home 	12010	nic Analysi	• •
TI DT426		169	600
		Range General-p	urpose
	THD-F : 5	51% THD-R:5.	50%
		<i>w</i>	
Ĩ.,	3		
» /	by		
» /	1		
/		1	
•		1	1
10			1
		2	کم
-09		2	~

View and verify waveforms on your mobile device like on an oscilloscope

Preserver (000 trape (Concernment) THOP 5245 THOP 5245 THOP 5245 1 17.60 2 0.28 3 0.40 4 0.13 5 0.61	14:09 TI DT4261		169		(**
1: 17.60 2: 0.28 3: 0.40 4: 0.13 5: 0.61					
2: 0.28 3: 0.40 4: 0.13 5: 0.61		THD-F : 5.7	4% THD-R: 5.3	73% 1	
3: 0.40 4: 0.13 5: 0.61			1:	17.60	1
4: 0.13 5: 0.61			2:	0.28	1
5: 0.61			3:	0.40	,
~			4:	0.13	1
~			5:	0.61	1
	Ś		^		
	50				

Screen 3

Troubleshoot with simple harmonic analysis in the field



 Save data and create reports right on the App
 Share data via cloud services or E-mail

Measurement up to CAT III 2000 V with the DC High Voltage Probe P2000 in Combination with DT4261

Safe Inspection of Solar Installations with High Voltage

Photovoltaic power generation equipment are becoming increasingly high-voltage in order to reduce costs and improve the efficiency of power generation systems. As a result, it is important to select measuring instruments that support higher voltage measurement to protect the safety of inspection workers.

DC HIGH VOLTAGE PROBE P2000 *Sold separately

Safe testers that protect workers from dangerous accidents

Built-in voltage input terminal protection fuse to prevent internal short circuits



The DT4255's voltage input terminals incorporate a protective fuse so that contamination of the instrument's internal components with iron powder or other particulate matter will not result in an internal short-circuit. The fuse can be replaced easily on site.

Terminal shutter to prevent accidental insertion






A range: Only the A and COM terminal inlets open. V range: Only the V and COM terminal inlets open.

The DT4281, DT4282 and DT4261 use terminal shutters to keep probes from being inserted into the wrong inlets. The shutters block whichever terminal is not being used based on the selected measurement function.

Equipped with a protection circuit to prevent accidents from incorrect voltage input







Over-input warning function




To prevent an accident, a warning function immediately notifies the operator if the DMM receives excessively high input.

*Red screen available on high-end models and DT4261, DT4223, DT4224 only.

Current measurement by AC clamp sensors to prevent accidents




The DT4281, DT4261, DT4253, DT4255 and DT4256 eliminate the root cause of such accidents by providing clamp-on sensor-based current measurement functionality instead of using conventional probes.



The DT4223 and DT4224 are equipped with a protection circuit that prevents electrical accidents that occure when voltage is input in the resistance range. The measurement circuit is switched after the instrument detects resistance, continuity, capacitance, or diode input. Even if you mistakenly input voltage with the instrument set to the resistance range, the high input impedance will limit the current flowing to the instrument to 1.5 mA or less to prevent potential hazards.



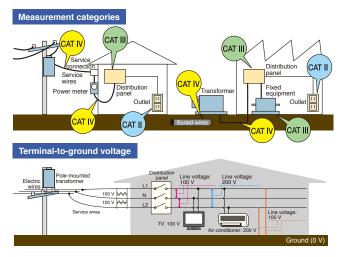


Safe measurement requires use of an instrument that suits the measurement location.

To ensure operators' ability to use measuring instruments safely, IEC 61010 classifies the locations in which instruments are used into a series of safety-based measurement categories (ranging from CAT II to CAT IV). Using an instrument that does not satisfy the required safety level can lead to an electrical accident.

AT IV 600 V

Terminal-to-ground voltage Measurement category suited to the location of use

High-end models	CAT III 1000 V / CAT IV 600 V
New Standard Model	CAT III 1000 V / CAT IV 600 V
Standard models	CAT III 1000 V / CAT IV 600 V
Pocket models	CAT III 600 V / CAT IV 300 V





All development, design, and manufacturing processes for almost all Hioki digital multimeters are carried out at our Head Office in Nagano Prefecture. Some of the industry's most advanced technological capabilities enable us to deliver products of the highest possible quality.





Field-Proven Strength and Usability DT4200 series

Robust design capable of withstanding a drop from a height of 1 m onto concrete



To test our products' ability to withstand mechanical shock, we repeatedly drop them from a height of at least 1 m until they break. This drop-testing regime leads to more robust products by fostering a series of design improvements.



Fast, accurate measurement of the output voltage on the secondary side of an inverter



The DT series can accurately measure the voltage on the secondary side of an inverter, just like a power meter. Its low-pass filter rejects harmonic components so that the fundamental wave can be isolated and accurately measured.

Outstanding viewing angle so display is easy to read at an angle or even in a dim location



The DT4200 series features a display with a wide viewing angle and a backlight function so that it's easy to read, even when you can't view the screen from the front or when making measurements in a dim location.

Hand-free and easy to use



It's hard to carry out work tasks smoothly when you're juggling a measuring instrument, probes, recording paper, and other supplies. Field concerns like these are resolved by the DT4200's magnetic strap, auto-hold function*, and ability to save results in its internal memory. These capabilities boost work efficiency and help reduce work times.

*The auto-hold function is available exclusively in high-end, standard models and DT4261,DT4223,DT4224. The ability to save results in internal memory is available exclusively in high-end models.

Preventing instrument failure by keeping out dust



If dust gets into the instrument's enclosure, it can cause the device to fail. Since dust can get into the instrument especially easily through the gap around the rotary switch, the DT4200 series incorporates a dust-proof part known as an O-ring where the rotary switch is mounted to improve the device's dust resistance.

True RMS measurement for accurate measurement of even distorted current waveforms




Current waveforms are often distorted, causing the average-value and true RMS measurement methods to yield different results. To obtain accurate readings, RMS measurement is indispensable.

Rotary switch that's easy to operate even when wearing gloves



The DT4200's rotary switch is designed to be easy to turn even when wearing thick work gloves, for example while working in hazardous measurement locations or harsh conditions.

New L9300 test leads with integrated cap*



Test leads L9300 now incorporate integrated caps. The design lets you change the measurement category simply by sliding the test lead's protective finger guard. As an added bonus, you no longer have to worry about losing caps!

*Standard accessory for DT4261

Extensive selection of probe tips that you can choose based on the measurement location, improving ease of measurement



With screw terminals



In deep-set locations that can't be reached with other probes



For clamping around the target busbar

With the DT4200, you can choose the probe type that best suits your measurement location, making it possible to measure in areas that can't be reached with conventional probes and busbars that you wish to clamp between probes.

*Compatible probe tips vary with the DMM model. Please see page 16. The optional Connection Cable L4930 is required in order to use the probes shown at the left.



High-end models

Featuring high accuracy, extensive additional functionality, and a broad range of measurement parameters

> DC V typical accuracy: ±0.025% rdg. ±2 dgt. Measurement categories: CAT III (1000 V), CAT IV (600 V)



For electrical work in the field DT4281

Designed for maximum safety in the field when measuring current with clamp-on sensors.

DC voltage	60.000 mV to 1000.0 V
AC voltage	60.000 mV to 1000.0 V
DC + AC voltage	6.000 V to 1000.0 V
DC current	600.00 µA to 600.00 mA
AC current	600.00 μA to 600.00 mA
AC clamp-on measurement	Frequency
AC clamp-on measurement Resistance	Frequency Continuity check
Resistance	Continuity check



For laboratory and research use DT4282

Designed for use in laboratories and R&D applications where you wish to measure a wide variety of parameters.

DC voltage	60.000 mV to 1000.0 V
AC voltage	60.000 mV to 1000.0 V
DC + AC voltage	6.000 V to 1000.0 V
DC current	600.00 µA to 10.000 A
AC current	600.00 μA to 10.000 A
AC clamp-on measurement	Frequency
AC clamp-on measurement Resistance	Frequency Continuity check
Resistance	Continuity check

Supported measurement parameter
 Supported measurement parameter (with model-specific variations)
 Unsupported measurement parameter
 *The range figures given indicate the instrument's measurement ranges (not the range of measurable values).

Functions and Features



Magnetic strap frees both hands for work Using the magnetic strap (option)

By using the magnetic strap to secure the instrument to the wall, you can free both hands so that you can more easily record measured values, significantly boosting work efficiency.



Automatically hold display values and save results with one touch to the DMM's internal memory

The display is automatically held once the measured value stabilizes. You can save measurement results to the instrument's internal memory simply by pressing the MEM key, making it easy to read and record values during inspection work.



Manage measurement data on a computer

Using the Communication Package DT4900-01 (option) Measurement results can be downloaded to a computer via a USB connection. Once downloaded, you can save them as a file (text format) or display them as a graph using the desired interval. Results can also be sent in real time while measurement is ongoing.

*The computer and multimeter are electrically isolated by means of optical communications so that data can be sent with peace of mind.




Measure output voltage on the secondary sides of inverters


Accurately measure the fundamental wave alone by eliminating harmonic components with the DMM's low-pass filter function.



Ripple voltage confirmation of DC charging systems Peak value measurement / DC + AC voltage measurement

High-end models can detect ripple voltage with a superposed DC signal.








Measure very low currents used by gas-burning devices DC µA range

High-end models provide a DC 600.00 µA range for measuring burner flame currents.





Intuitive notification of continuity check results and excessively high input with a red screen backlight and beep

High-end models notify the operator of continuity check results and excessively high input with a red screen backlight and beep, making it possible to check measurement results intuitively





Excessively high input



instrumentation signal measurement 4 to 20 mA / 0 to 20 mA percentage-

Output 1

Display

0%

0%

You can check percentage-equivalent

Percentage display for

equivalent display

values



SLOW ANGE: AUTO **Display refresh rate**

Change the display refresh speed to stabilize the display when performing measurement characterized by a high level of variability



Transducer

Maximum/minimum

Check the maximum and minimum measured values shown on the display after pressing the MAX/MIN button



Relative display

View relative values using the display value before the relative function was enabled as the reference.



value display



Decibel conversion

Convert the results of AC voltage measurement to a decibel value relative to a reference value and display the results (dbm/ dby)

7



New standard model

Supports wireless communication to increase work efficiency. High voltage measurement up to CAT III 2000 V by connecting a dedicated probe.

> DC V typical accuracy: ±0.15% rdg. ±2 dgt. Measurement categories: CAT III (1000 V), CAT IV (600 V)

Safe Inspection of Solar Installations with High Voltage



By connecting the optional DC High Voltage Probe P2000, high voltage measurement up to CAT III 2000 V is now possible.

Why is CAT III 2000 V capability necessary?

According to the standards for Photovoltaic (PV) module safety qualification (IEC 61730-1), PV modules are treated as the overvoltage category III, and a measuring instrument in the measurement category III is required. Using instruments that can accommodate the appropriate measurement category serves to protect workers and equipment from serious accidents such as electric shock and burnout.Currently, adoption of 1500 V solar installation is growing, but instruments that can accommodate even higher voltages will be necessary in the future as larger and even more efficient systems enter into use.



Multi-functional, on-site maintenance, mega solar **DT4261**

Go wireless with the Z3210! For trouble analysis in the field.

DC voltage	600.0 mV to 1000 V
AC voltage	6.000 V to 1000 V
DC + AC voltage	6.000 V to 1000 V
DC current	600.0 mA to 10.00 A
AC current	600.0 mA to 10.00 A
AC clamp-on measurement	Frequency
AC clamp-on measurement Resistance	Frequency Continuity check
Resistance	Continuity check

Easily go wireless and manage your data digitally

WIRELESS ADAPTER Z3210



Wireless communication is supported in combination with the wireless adapter Z3210 (sold separately). In addition to working with the free "GENNECT Cross" application, the Excel® direct input function can also be used.

NEW DT4261-90 (Z3210 set product)

The DT4261-90, a set of DT4261 and Z3210, is also available. It is more economical than purchasing the DT4261 and Z3210 separately, and allows you to build a wireless communication environment with one purchase.

🚯 Bluetooth



Supported measurement parameter
 Unsupported measurement parameter

*The range figures given indicate the instrument's measurement ranges. Not the range of measurable values. Please see page 16 for details.

Link with GENNECT Cross



Troubleshoot in the field

When combined with GENNECT Cross, the DT4261 you can perform simple harmonic analysis. Applications include harmonic measurement of power conditioners for solar systems and problem analysis of power supply systems.

Problems that can be caused by harmonics

- · Equipment burn-out and destruction due to overheating
- Malfunctions of power control devices
- · Reduced service life and efficiency for power devices

Excel[®] Direct Input Function

HIOKI Z3210	8	Blu)) ietoo	oth	X	
HIC	Ж	Title		DEMO		Person in charg
Company name	HIOKI	DATE EMPERATUR *C	HUMIDITY			
	HIOKI Insulation resistance value	EMPERATUR			Unit	Judgement
	Insulation	EMPERATUR °C	HUMIDITY	JLF	Unit	Judgement
Company name	Insulation resistance value		HUMIDITY	Current value		
Company name	Insulation resistance value 101	EMPERATUR °C Unit M Ohm	HUMIDITY Judgement PASS	Current value 3.11	A	PASS

Improve work efficiency! Labor-saving measurement with digitalization

The wireless adapter Z3210 (sold separately) comes standard with an Excel® direct input function. It enables direct transfer and input of measurement data to templates created in Excel® leading to increased work efficiency in the field.

Functions and Features





Terminal shutter closes on unused terminals depending on the measurement function

The DT4261's terminal shutters are linked to the instrument's rotary switch. They block access to test lead terminals that aren't being used, making it physically impossible to insert a lead into the wrong terminal.



Test leads with an integrated cap for greater convenience and safety

The L9300 test lead with an integrated cap is included as a standard. The finger guard can be easily slid to switch between measurement categories without worrying about losing the cap.



Prevents incorrect current measurement with the Fuse Check function

When switching from the clamp function to the current function, a fuse disconnection check is automatically performed. This allows the user to know if the fuse is broken before current measurement, which prevents erroneous measurement.



Free up hands for work with the magnetic strap* and auto-hold function *The Magnetic Strap is sold separately

By using the magnetic strap to secure the instrument to the wall and the auto-hold function to automatically stop display values, you can free your hands, making it easier to record measured values and significantly boosting work efficiency.




Automatic switching of measurement in locations where AC and DC voltages are mixed

When making measurements in locations with both AC and DC voltages, automatic switching eliminates the need to operate the rotary switch and helps prevent measurement mistakes.



Manage measurement data on a computer Using the Communication Package DT4900-01 (sold separately)

Measurement results can be downloaded to a computer via a USB connection. Once downloaded, you can save them as a file (text format) or display them as a graph using the desired interval. Results can also be sent in real time while measurement is ongoing.

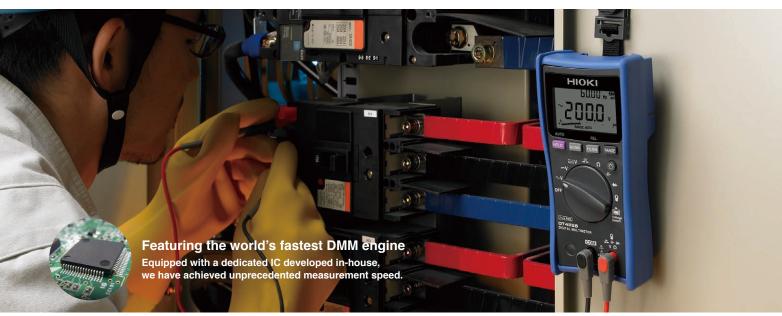

Standard models

Introducing a line of field-optimized instruments that can be chosen based on the application at hand DC V typical accuracy: ±0.3% rdg. ±3 dgt.

Measurement categories: CAT III (1000 V), CAT IV (600 V)



For laboratory and research use **DT4252**

For laboratories and R&D applications where you wish to measure a wide variety of parameters.

DC voltage	600.0 mV to 1000 V
AC voltage	6.000 V to 1000 V
DC + AC voltage	DT4281/4282 only
DC current	6.000 A to 10.00 A
AC current	6.000 A to 10.00 A
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic	Voltage detection



For instrumentation 4-20 mA **DT4253**

Measure instrumentation, airconditioning equipment, and gas-burning devices.

DC voltage	600.0 mV to 1000 V
AC voltage	6.000 V to 1000 V
DC + AC voltage	DT4281/4282 only
DC current	60.00 µA to 60.00 mA
AC current	
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic	Voltage detection



For electrical work in the field **DT4255**

Designed for maximum safety with voltage measurement terminals that are protected by a fuse.

DC voltage	600.0 mV to 1000 V
AC voltage	6.000 V to 1000 V
DC + AC voltage	DT4281/4282 only
DC current	n/a
	n/a
AC clamp-on	Frequency
measurement	Frequency
Resistance	Continuity check
Resistance	Continuity check



model **DT4256**

Delivers maximum functionality for use in a wide range of settings.

DC voltage	600.0 mV to 1000 V
AC voltage	6.000 V to 1000 V
DC + AC voltage	DT4281/4282 only
DC current	60.00 mA to 10.00 A
AC current	600.0 mA to 10.00 A
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic detection	Voltage detection function

Supported measurement parameter Supported measurement parameter (with model-specific variations) Unsupported measurement parameter The range figures given indicate the instrument's measurement ranges (not the range of measurable values).

*Your instrument can be used to measure voltages in excess of 1000 V DC if and only if both of the following conditions are satisfied: 1. The circuit under measurement is isolated from the commercial power grid. 2. The circuit under measurement is isolated from ground.

Functions and Features



Magnetic strap and auto-hold function free up hands for easier work

Using the magnetic strap (option)

By using the magnetic strap to secure the instrument to the wall and the auto-hold function to automatically stop display values, you can free your hands, making it easier to record measured values and significantly boosting work efficiency.



Automatic switching of measurement in locations where AC and DC voltages are mixed AC/DC voltage automatic detection (DT4253, DT4255, DT4256 only)

When making measurements in locations with both AC and DC voltages, automatic switching eliminates the need to operate the rotary switch and helps prevent measurement mistakes.



Use a computer in the field to save and check measured values With the Communication Package DT4900-01 (option)


Measured values can be displayed in real time on a computer, and displayed values can be saved to a file (text format) or graphed at a user-specified interval.

*The computer and multimeter are electrically isolated by means of optical communications so that data can be sent with peace of mind.



Measure output voltage on the secondary sides of inverters

Accurately measure the fundamental wave by eliminating harmonic components with the DMM's low-pass filter function.





Over-input warning function

To prevent an accident, a warning function immediately notifies the operator if the DMM receives excessively high input.

Polarity detection and notification

Certain standard models can detect a load voltage in excess of -10 V and notify the operator with a red LED and beep. (DT4255, DT4256 only)





Percentage display for

instrumentation signal measurement 4 to 20 mA percentage-equivalent display (DT4253 only) The standard models' dual display function lets you to simultaneously check measured values and percentage-equivalent values at a glance.





Measure very low currents used by gas-burning devices DC µA range (DT4253 only)

Model DT4253 provides a DC 60.00 µA range for measuring burner flame currents.





Intuitive notification of continuity check results and excessively high input with a red LED and beep


Standard models notify the operator of continuity check results and excessively high input with a red LED and beep, making it possible to check measurement results intuitively.




Continuous state Excessively high input

Thorough prevention of shortcircuit accidents

Voltage measurement terminal fuse (DT4255 only) When using the resistance measurement function, a protective circuit functions to prevent a short-circuit accident in the event of erroneous operation such improperly supplying voltage input. Even if a short-circuit occurs inside the tester, a current-limiting resistor will limit any short-circuit current while a fast-blow fuse quickly and reliably disconnects the tester circuitry, preventing a short-circuit accident.



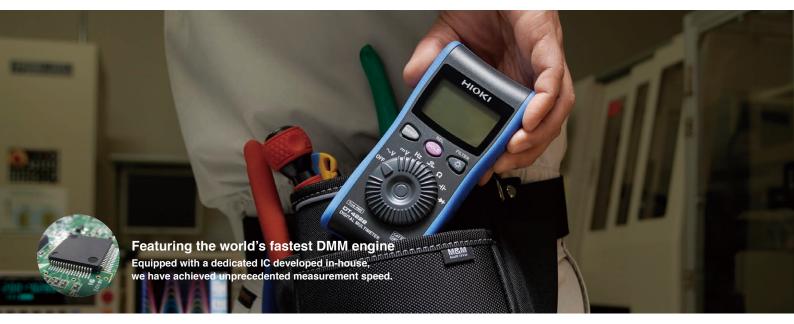

Pocket models

Featuring a compact body for ergonomic hold and a reliable, safe design





For electrical work in the field DT4221

Delivering maximum field safety for workers whose principal use is voltage measurement.

DC voltage	600.0 mV to 600.0 V
AC voltage	6.000 V to 600.0 V
DC + AC voltage	DT4281/4282 only
DC current	n/a
AC current	n/a
AC clamp-on measurement	Frequency
	Continuity check
Temperature	Diode test
	Conductance
AC/DC automatic	Voltage detection



For multiple applications DT4222

For laboratories and R&D applications to measure a wide variety of parameters.

DC voltage	600.0 mV to 600.0 V
AC voltage	6.000 V to 600.0 V
DC + AC voltage	DT4281/4282 only
DC current	n/a
AC current	n/a
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic detection	Voltage detection function

For electrical work in the field DT4223

HIOK

Delivering maximum field safety for workers whose principal use is voltage measurement.

DC voltage	600.0 mV to 600.0 V
AC voltage	6.000 V to 600.0 V
DC + AC voltage	DT4281/4282 only
DC current	n/a
AC current	n/a
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic	Voltage detection



For multiple applications DT4224

For laboratories and R&D applications to measure a wide variety of parameters.

DC voltage	600.0 mV to 600.0 V
AC voltage	6.000 V to 600.0 V
DC + AC voltage	DT4281/4282 only
DC current	n/a
AC current	n/a
AC clamp-on measurement	Frequency
Resistance	Continuity check
Temperature	Diode test
Capacitance	Conductance
AC/DC automatic	Voltage detection

Supported measurement parameter
 Supported measurement parameter (with model-specific variations)
 Unsupported measurement parameter
 *The range figures given indicate the instrument's measurement ranges (not the range of measurable values).

Functions and Features

New DT4223 and DT4224 feature circuit breaker false trip prevention



Prevent potential accidents during incorrect input

The measurement circuit switches only after detecting the appropriate signal. This way, even if you mistakenly input voltage, accidents due to tripped breakers or arcs will not happen. (see page 2)



LoZ icon identifies switched measurement circuit

When the instrument detects resistance, continuity, capacitance, or diode input, the LoZ icon is shown on the display, allowing you to identify at a glance which measurement circuit has been selected.



Warning function notifies you of incorrect input. The instrument's display flashes red to warn you when voltage has been mistakenly input while the instrument is set to the resistance range.



Compact and lightweight design for outstanding ease of use

The small form factor fits in your hand perfectly and is easily stowable, making it convenient to transport to and from the field and boosting work efficiency. The lightweight design also ensures that pocket models are easy to work with.



Safe enough for measuring voltage at distribution panels and service wires

Despite a compact body, the pocket models can be used to measure voltage at distribution panels and service wires in CAT III (600 V), CAT IV (300 V) situations.



Intuitive notification of excessively high input with flashing screen

The pocket digital multimeters notify the operator of excessively high input by flashing the screen, making it possible to check measurement results intuitively.



Automatic switching of measurement in locations where AC and DC voltages are mixed

AC/DC voltage automatic detection (DT4221, DT4223 only) When making measurements in locations with both AC and DC voltages, automatic switching eliminates the need to operate the rotary switch and helps prevent measurement mistakes





Detect voltage simply by holding the instrument against a wire

Voltage detection function (DT4221, DT4223 only)

Easily detect voltage with the built-in sensor. Results are communicated with a beep.







DT4221

ease of use

measurement results Fast measurement for outstanding

Measured values are displayed quickly to facilitate quick testing. The difference is clear when you compare the measurement speed with that of the Hioki Card HiTESTER 3244-60.

DT4200 Series Basic Comparison

Model category	High-end models	New standard models		Standard	models			Pocket r	nodels	
Measurement type	Electrical General work use	General use/ mega Solar	General use	Air conditioning/ instrumentation	Electrical work	General use	Electrical work	General use	Electrical work	General use
Model	DT4281 DT4282	DT4261/DT4261-90*1	DT4252	DT4253	DT4255	DT4256	DT4221	DT4222	DT4223	DT4224
Appearance										
Basic Characteristic	S									
True RMS	<i>v</i>	 ✓ 		~	,			~		
DC V basic accuracy	±0.025% rdg. ±2 dgt.	±0.15% rdg. ±2 dgt.	±0.3% rd	g. ±5 dgt.	±0.3% r	dg. ±3 dgt.		±0.5% rdg	. ±5 dgt.	
Measurement items	(Typical ranges are indicate	ed; may not reflect maxi	mum or minin	num measurab	le signal)					
DC voltage	60 mV to 1000 V	600 mV to 1000 V, 2000V*2		600 mV to	o 1000 V			600 mV t	600 V	
AC voltage	60 mV to 1000 V	6 V to 1000 V		6 V to	600 V			6 V to 6	00 V	
DC V + AC V	6 V to 1000 V	6 V to 1000 V		n/	a			n/a	L	
DC A current	600 µA to 600 mA 600 µA to 10 A	600 mA to 10 A	6 A to 10 A	60 µA to 60 mA	n/a	60 mA to 10 A		n/a	L	
AC A current	600 µA to 600 mA 600 µA to 10 A	600 mA to 10 A	6 A to 10 A	n/	a	600 mA to 10 A		n/a	L	
AC clamp	10 A to 1000 A n/a	10 A to 1000 A	n/a		10 A to 1000 A	4		n/a	L	
Resistance	60 Ω to 600 MΩ	600 Ω to 60 MΩ		600 Ω to	60 MΩ		n/a	60	0 Ω to 60 I	NΩ
Temperature	-40°C to 800°C	n/a	n/a	-40°C to 400°C	ı	n/a		n/a	L	
Capacitance	1 nF to 100 mF	1 µF to 10 mF		1 μF to	10 mF		n/a	1 µF to 10 mF	n/a	1 µF to 10 mF
Frequency	99 Hz to 500 kHz	99 Hz to 99 kHz		99 Hz to	99 kHz			99 Hz to	9.9 kHz	
Continuity check	V	~		V	,			~		
Diode check	~	~		~	,		n/a	v	n/a	~
Conductance	n/a 🖌	n/a		n/	a			n/a	L	
Voltage detection	n/a	n/a	n	/a		v	~	n/a	~	n/a
Additional Functions	3		1	1						
AUTO AC/DC V	n/a	V	n/a		~		V	n/a	~	n/a
Peak measurement	DC/AC	DC/AC		n/				n/a		
Low-pass filter	Analog filter Cut-off: 630 Hz	Digital filter Pass-band: 100/500 Hz		Digital Pass-band:	100/500 Hz			Digital Pass-band: 1	00/500 Hz	
Display update setting		n/a		n/				n/a		
Hold display value	AUTO/MANUAL	AUTO/MANUAL		AUTO/M			MAI	NUAL		/MANUAL
Max/Min value display	 (Excluding average value display) 	v		~				n/a	L	
Relative display Decibel conversion	<i>v</i>	n/a		v				V		
	~	n/a n/a	n/a	n/		n/a		n/a n/a		
Percentage conversion display DC voltage polarity check	~	n/a n/a		∕a		√		n/a n/a		
Data storage	•	100		~		-		11/c		
Capacity	Max 400 data	n/a		n/	a			n/a		
USB communication* ³	✓	✓		· · · · ·				n/a		
Bluetooth® communication*4	n/a	V		n/				n/a		
Operating time										
Continuous operating time	Approx. 100 hours* ⁵	Approx. 130 hours*6		Approx. 1	30 hours		Approx.	40 hours	Approx	. 35 hours
Power supply	Alkaline (LR6) battery ×4/ Manganese(R6P) battery ×4	Alkaline (LR6) battery ×3		Alkaline (LR0		1		Alkaline (LR03) battery ×	1
Display		i 	·							
Back light	✓	<i>v</i>		~	,			<i>~</i>		
Dual display	V	~		V				n/a		
Bar graph display	n/a	~		~	,			V		
Safety										
	CAT III 1000 V, CAT IV 600 V	CAT III 1000 V, CAT IV 600 V		CAT III 1000 V,	CATIV 600 \	/		CAT III 600 V, 0	ATIV 300	V
Mis-insertion prevention shutters	v	~		n/				n/a		
Circuit breaker false trip prevention	n/a	n/a		n/s	a		r	ı/a		~

*1. Z3210 set product *2. 2000 V is supported only when using the optional DC HIGH VOLTAGE PROBE P2000 *3. Requires optional DT4900-01 Communication Package *4. Requires optional Z3210 wireless adapter *5. When using four AA alkaline batteries *6. When Z3210 is not installed

Glossary

Auto AC/DCV : Automatically detects and measures AC and DC voltage. I Peak measurement : After starting PEAK value measurement, check maximum and minimum instantaneous voltage and current values. I Low-pass filter : Cuts high frequency content to provide stable numerical values for measurement. I Display update setting : Reduces the display value update rate to stabilize measurements. I Hold display value : Manual: press the button to freeze the display. Auto: the display freezes automatically when the measurement value is stable. | Max/Min value display : Pressing the MAX/MIN button displays the maximum and minimum displayed measurement values. I Relative display : Pressing the REL button displays subsequent measurements as values relative to that displayed when the button was pressed. I Decibel conversion : Displays AC voltage measurements converted to decibel values (dbm/dbv) | Percentage conversion display : Displays 4 to 20 mA (or 0 to 20 mA) signals converted to 0 to 100% values. For the DT4253, only 4 to 20 mA.

High-End DT4281 / DT4282 (Accuracy guaranteed for 1 year)

DC Voltage		
Range	Accuracy	Input Impedance
60.000 mV	±0.2% rdg. ±25 dgt.	1 GΩ or more // 100 pF or less
600.00 mV	±0.025% rdg. ±5 dgt.	1 Gizz of filore // 100 pF of less
6.0000 V	0.005% rda0 dat	11.0 MΩ ±2% // 100 pF or less
60.000 V	±0.025% rdg. ±2 dgt.	10.3 MΩ ±2% // 100 pF or less
600.00 V	±0.03% rdg. ±2 dgt.	10.2 MΩ ±2% // 100 pF or less
1000.0 V	±0.05% rdg. ±2 dgl.	10.2 W12 ±2 % // 100 pF or less

AC Volt	AC Voltage						
Panga		Accuracy					
Range	20 Hz to 45 Hz	45 Hz to 65 Hz	65 HZ to 1 kHz	1 kHz to 10 kHz	10 kHz to 20 kHz	20 kHz to 100 kHz	
60.000 mV	±1.3% rdg.	±0.4% rdg.	±0.% rdg.	±0.9% rdg.	±1.5% rdg.	±20% rdg. ±80 dgt.	
600.00 mV	±60 dgt.	±40 dgt.	±40 dgt.	±40 dgt.	±40 dgt.	±8% rdg. ±80 dgt.	
6.0000 V	±1% rdg. ±60 dgt.				±0.7% rdg. ±40 dqt.	±3.5% rdg. ±40 dqt.	
60.000 V		±0.2% rdg. ±25 dqt.	±0.3% rdg. ±25 dgt.	±0.4% rdg. ±25 dgt.	±40 ugi.	±40 ugi.	
600.00 V	Undefined	±25 ugi.			Undefined	Undefined	
1000.0 V					Undelined	Undelined	

DC V +	DC V + AC V Measurement					
Range			Ac	curacy		
nange	20 Hz to 45 Hz	45Hz to 65Hz	65 HZ to 1 kHz	1 kHz to 10 kHz	10kHz to 20kHz	20 kHz to 100 kHz
6.0000 V	±1.2% rdg. ±65 dgt.			±0.4% rdg.	±1.5% rdg. ±45 dqt.	±3.5% rdg. ±125 dgt.
60.000 V		±0.3% rdg.	±0.4% rdg.	±30 dgt.	140 ugi.	120 ugi.
600.00 V	Undefined	±30 dgt.	±30 dgt.			
1000.0 V	ondenned			±0.4% rdg. ±45 dgt.	Undefined	Undefined
Input impe	dance	1 MΩ ±4%	// 100 pF or le	ess		
Crest facto	Crest factor 3 or less (1.5 or less for the 1000.0 V range)					
5% or more of each range						
Accuracy specification range With the filter ON, accuracy is defined only for frequencies 100 Hz or less. Furthermore, 2% rdg. is added.				encies		

DC A Meas	surement	*-	1. DT4282 only
Range	Accuracy / Display update : slow	Accuracy / Display update : normal	Shunt Resistance
600.00 μA		±0.05% rdg. ±25 dgt.	101 Q
6000.0 µA	±0.05% rdg. ±5 dgt.	±0.05% rdg. ±5 dgt.	101 12
60.000 mA		±0.05% rdg. ±25 dgt.	10
600.00 mA	±0.15% rdg. ±5 dgt.	±0.15% rdg. ±5 dgt.	1 1 1 2
6.0000 A*1	10.0% rda 15 dat	±0.2% rdg. ±25 dgt.	10 mQ
10.000 A*1	±0.2% rdg. ±5 dgt.	±0.2% rdg. ±5 dgt.	10 m22

asurement	*1.	DT4282 only		
20 Hz to 45 Hz	45 Hz to 65 Hz	65 Hz to 1 kHz	1 kHz to 10 kHz	10 kHz to 20 kHz
±1.0% rdg. ±20 dgt.	±0.6% rdg. ±20 dgt.	±0.6% rdg. ±20 dgt.	±2% rdg. ±20 dgt.	±4% rdg. ±20 dgt.
±1.0% rdg. ±5 dgt.	±0.6% rdg. ±5 dgt.	±0.6% rdg. ±5 dgt.	±2% rdg. ±5 dgt.	±4% rdg. ±5 dgt.
±1.0% rdg. ±20 dgt.	±0.6% rdg. ±20 dgt.	±0.6% rdg. ±20 dgt.	±1% rdg. ±20 dgt.	±2% rdg. ±20 dgt.
±1.0% rdg. ±5 dgt.	±0.6% rdg. ±5 dgt.	±0.6% rdg. ±5 dgt.	±1.5% rdg. ±10 dgt.	Undefined
Undefined	±0.8% rdg. ±20 dgt.	±0.8% rdg. ±20 dgt.	Undefined	Undefined
Undefined	±0.8% rdg. ±5 dgt.	±0.8% rdg. ±5 dgt.	Undefined	Undefined
Shunt resistance μ A Range 101 Ω , mA Range 1 Ω , A Range 10 m Ω				Ω
Crest factor 3 or less (Note that it applies to 1/2 of the range.))
	20Hz to 45 Hz ±1.0% rdg. ±20 dgt. ±1.0% rdg. ±5 dgt. ±1.0% rdg. ±20 dgt. ±1.0% rdg. ±5 dgt. Undefined Undefined	20Hz to 45 Hz 45Hz to 65 Hz ±1.0% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±1.0% rdg. ±0.6% rdg. ±5 dgt. ±5 dgt. ±20 dgt. ±0.6% rdg. ±5 dgt. ±5 dgt. ±1.0% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±1.0% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±1.0% rdg. ±2.6% rdg. ±20 dgt. ±20 dgt. ±0.6% rdg. ±2.6% rdg. ±5 dgt. ±20 dgt. Undefined ±0.8% rdg. ±5 dgt. ±5 dgt. undefined ±0.8% rdg. ±5 dgt. ±6 dgt.	Accuracy 20Hz to 45 Hz 45Hz to 65 Hz 65Hz to 1 kHz ±1.0% rdg. ±0.6% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±20 dgt. ±1.0% rdg. ±0.6% rdg. ±20 dgt. ±5 dgt. ±5 dgt. ±5 dgt. ±1.0% rdg. ±0.6% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±20 dgt. ±1.0% rdg. ±0.6% rdg. ±0.6% rdg. ±20 dgt. ±20 dgt. ±20 dgt. ±1.0% rdg. ±0.6% rdg. ±0.6% rdg. ±1.0% rdg. ±0.6% rdg. ±0.6% rdg. ±5 dgt. ±5 dgt. ±5 dgt. undefined ±0.8% rdg. ±0.8% rdg. ±0.8% rdg. ±5 dgt. ±5 dgt. undefined ±0.8% rdg. ±5 dgt. ±5 dgt. ±5 dgt. ±5 dgt.	$\begin{tabular}{ c c c c } \hline & & & & & & & & & & & & & & & & & & $

Accuracy specification range Accuracy is not defined for measurements below 5% of range

Continuity Check			
Range	Accuracy	Measurement Current	Open-terminal Voltage
600.0 Ω	±0.5% rdg. ±5 dgt.	640 μA ±10%	DC 2.5 V or less
Continuity threshold	20 Ω (default), 50 Ω,	100 Ω, 500 Ω	

Diode Check					
Range		Accuracy	Measurement Current	Open-terminal Voltage	
3.600 V	±0.1% rdg. ±5 dgt.		1.2 mA or less	DC 4.5 V or less	
Forward threshold	1	If the reading is lowe	lt), 1 V, 1.5 V, 2 V, 2.5 r than the threshold d	uring the forward con-	
		nection, a buzzer sounds and the red backlight turns on.			

AC Clamp (AC Current) DT4281 onl						
Danga	Acc	curacy				
Range	40 Hz to 65 Hz	65 Hz to 1 kHz				
10.00 A	±0.6% rdg. ±2 dgt.	±0.9% rdg. ±2 dgt.				
20.00 A	±0.6% rdg. ±4 dgt.	±0.9% rdg. ±4 dgt.				
50.00 A	±0.6% rdg. ±10 dgt.	±0.9% rdg. ±10 dgt.				
100.0 A	±0.6% rdg. ±2 dgt.	±0.9% rdg. ±2 dgt.				
200.0 A	±0.6% rdg. ±4 dgt.	±0.9% rdg. ±4 dgt.				
500.0 A	±0.6% rdg. ±10 dgt.	±0.9% rdg. ±10 dgt.				
1000 A	±0.6% rdg. ±2 dgt.	±0.9% rdg. ±2 dgt.				
	0-50, 9018-50, or 9132-50 CLAMP tot include the error of the clamp-on					
Crest factor	st factor 3 or less					
Accuracy is not defined for measurements below 15% of range						
-						

Resistance Measurement					
Range	Accuracy	Measurement Current	Open-terminal Voltage		
60.000 Ω	±0.3% rdg. ±20 dgt.	640 μA ±10%			
600.00 Ω	±0.03% rdg. ±10 dgt.	040 μA ±10%			
6.0000 kΩ		96 μA ±10%			
60.000 kΩ	±0.03% rdg. ±2 dgt.	9.3 μA ±10%			
600.00 kΩ		0.96 μA ±10%	DC 2.5 V or less		
6.0000 MΩ	±0.15% rdg. ±4 dgt.				
60.00 MΩ	±1.5% rdg. ±10 dgt.	96 nA ±10%			
600.0 MQ	±3.0% rdg. ±20 dgt.	90 HA ±10%			
000.0 10122	±8.0% rdg. ±20 dgt.]			

Conductanc	e (nS)		DT4282 only
Range	Accuracy	Measurement Current	Open-circuit Voltage
600.00 nS	±1.5% rdg. ±10 dgt.	96 nA ±10%	DC 2.5 V or less

Accuracy is defined for humidity 60% RH or less. Accuracy is defined for the range 20nS or more. In the case of 300 nS or more, ± 20 dgt. is added.

Capacitance Measurement					
Range	Accuracy	Measurement Current	Open-circuit Voltage		
1.000 nF	±1% rdg. ±20 dgt.				
10.00 nF		32 μA ±10%	DC 2.5 V or less		
100.0 nF	±1% rdg. ±5 dgt.				
1.000 μF					
10.00 μF			DC 3.1 V or less		
100.0 μF	±2% rdg. ±5 dgt.		DC 3.1 V 01 less		
1.000 mF	±2% lug. ±5 ugi.	680 μA ±20%			
10.00 mF			DC 2.1 V or less		
100.0 mF	±2% rdg. ±20 dgt.				

Temperature				
Thermocouple Type	Range	Accuracy		
К	-40.0°C to 800.0°C (-40.0°F to 1472.0°F)	±0.5% rdg. ±3°C (5.4°F)		
The optional K Thermocouple DT4910 is used. Accuracy does not include the error of the K thermocouple.				

Frequency (For AC V, DC + AC V, AC µA, AC mA, AC A)			
Range	Accuracy		
99.999 Hz			
999.99 Hz	±0.005% rdg. +3 dgt.		
9.9999 kHz			
99.999 kHz	- 0.00E0(rdz		
500.00 kHz	±0.005% rdg. +3 dgt.		
Measurement ra	e 0.5 Hz or more ([] is displayed when frequency is less than 0.5 Hz)		
Pulse width 1 µs or more (DUTY ratio is 50%)			

With the filter ON, accuracy is defined only for frequencies 100 Hz or less. (For ACV, DC+ACV)

Peak Measurement (For AC V, DC V, DC+AC V, Clamp, DC µA, DC mA, DC A, AC µA, AC mA, AC A)				
Main measurement Signal width Accuracy				
DC V	4 ms or more (single)	±2.0% rdg. ±40 dgt.		
	1 ms or more (repeated)	±2.0% rdg. ±100 dgt.		
Other than DC V	1 ms or more (single)	±2.0% rdg. ±40 dgt.		
	250 µs or more (repeated)	±2.0% rdg. ±100 dgt.		

Decibel Conversion Measurement : Standard impedance (dBm	n)
--	----

4, 8, 16, 32, 50, 75, 93, 110, 125, 135, 150, 200, 250, 300, 500, 600, 800, 900, 1000, 1200 Ω (default: 600 $\Omega)$

High-End General Specifications

Durability					
Drop proof	Yes				
Operating temperature and humidity*1	-15°C to 55°C				
Storage temperature and humidity*2	-30°C to 60°C				
Applicable standards	Safety: EN61010, EMC: EN61326; Waterproof and dustproof: IP40				
*115°C to 55°C (5°F to 131°F), Up to 40°C (104°F): at 80% RH or less (non-condensating),					

40°C to 45°C (104°F to 113°F): at 60% RH or less (non-condensating), 45°C to 55°C (113°F to 131°F): at 50% RH or less (non-condensating)

*2. 80%RH or less (non-condensating)

Dimensions/Weight

93W × 197H × 53D mm (3.66"W × 7.76"H × 2.09"D), 650 g (23 oz.) (including batteries)

Safety Maximum rated voltage between CAT III 1000 V, CAT IV 600 V input terminals and ground CAT III 1000 V, CAT IV 600 V Maximum rated voltage between terminals Between the V and COM terminals: 1000 V DC/AC Maximum rated current between terminals Between the MA and COM terminals: 600 mA DC/600 mA AC Between the A and COM terminals: 10 A DC/10 A AC

Accessories

TEST LEAD L9207-10, Instruction Manual, LR6 alkaline battery × 4

.....

New Standard

NEW DT4261

(Accuracy guaranteed for 1 year)

DC Voltage					
Range	Accuracy*1	Input Impedance			
600.0 mV	±0.15% rdg. ±5 dgt.	11.3 MQ ± 2.0%			
6.000 V		11.3 IVIC2 ± 2.0%			
60.00 V	±0.15% rdg. ±2 dgt.	10.4 MΩ ± 2.0%			
600.0 V		10.3 MQ ± 1.5%			
1000 V	±0.15% rdg. ±5 dgt.	10.3 ML2 ± 1.5%			
2000 V*2	±0.5% rdg. ±5 dgt.	20 MΩ ± 5.0%			
*1. Add ±1 dat, when measuring at or below 5% of range					

*2. 2000 V is supported only when using the optional DC HIGH VOLTAGE PROBE P2000

AC Voltage						
D		Accuracy		Innut Imnodonoo		
Range	40 Hz to	500 Hz	500 Hz to 1 kHz	Input Impedance		
6.000 V				11.3 M Ω ± 2.0% // 100 pF or less		
60.00 V	±0.9% rdd	2 dat	±1.5% rdg. ±3 dgt.	10.4 MΩ \pm 2.0% // 100 pF or less		
600.0 V	±0.9% 100	J. ±3 üğι.		10.3 MΩ ± 1.5% // 100 pF or less		
1000 V				$10.3 \text{ M}\Omega \pm 1.3\% \text{ // }100 \text{ pr or less}$		
Crest factor		3 at up to 4000 counts and reduces linearly to 2 at 6000 counts. 1000 V range only: 2 at up to 750 counts, linearly decreasing to 1.5 at 1000 counts.				

Accuracy specification range For ACV, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range.

DC A Measurement				
Range	Accuracy	Input Impedance		
600.0 mA		35 mΩ ±30%		
6.000 A	±0.5% rdg. ±3 dgt.			
10.00 A				
Accuracy specification range Add ±2 dgt. when measuring at or below 5% of range.				

 AC A Measurement

 Range
 Accuracy
 Input Impedance

 600.0 mA
 500 Hz
 500 Hz to 1 kHz
 Input Impedance

 6.000 A
 ±1.4% rdg. ±3 dgt.
 ±1.8% rdg. ±3 dgt.
 35 mΩ ±30%

 Crest factor
 3 at up to 4000 counts and reduces linearly to 2 at 6000 counts.

 Accuracy specification range
 For ACV, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range.

Continuity Check					
Range	Ac	curacy	Measurement Current	Open-terminal Voltage	
600.0 Ω	±0.7% rdg. ±5 dgt.		Approx. 200 µA	DC 2.0 V or less	
Continuity ON threshold Approx. 25 Ω or less (continuous buzzer sound, red backlight on)					

Continuity OFF threshold Approx. 245 Ω or more (buzzer sound off, red backlight off)

Diode Check					
Range	Accuracy	Measurement Current	Open-terminal Voltage		
1.800 V	±0.5% rdg. ±5 dgt.	Approx. 200 µA	DC 2.0 V or less		
Forward threshold		ound at 0.15 V to 1.8 V 15 V, red backlight on.	/, continuous buzzer		

AC Clamp (AC Current)					
Dongo	Accuracy				
Range	40 Hz to 500 Hz	500 Hz to 1 kHz			
10.00 A					
20.00 A					
50.0 A					
100.0 A	±0.9% rdg. ±3 dgt.	±1.5% rdg. ±3 dgt.			
200.0 A					
500 A					
1000 A					
The optional 9010-50, 9018-50, or 9132-50 CLAMP ON PROBE is used. Accuracy does not include the error of the clamp-on probe.					
Crest factor	Crest factor 3 or less				

Accuracy specification range Minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range

Resistance Measurement					
Range	Accur	acy	Measurement Current	Open-terminal Voltage	
600.0 Ω	±0.7% rdg	. ±5 dgt.	Approx. 200 µA		
6.000 kΩ			Approx. 100 µA		
60.00 kΩ	±0.7% rdg	. ±3 dgt.	Approx. 10 µA	DC 2.0 V or less	
600.0 kΩ	1		Approx. 1 µA	DC 2.0 V or less	
6.000 MΩ	±0.9% rdg	. ±3 dgt.	Approx. 100 nA		
60.00 MΩ	±1.5% rdg	. ±3 dgt.	Approx. 10 nA		
Accuracy quarantee condition After zero adjustment has been performed					

Accuracy guarantee condition After zero adjustment has been performe

Capacitance Measurement				
Range	Accuracy	Measurement Current	Open-terminal Voltage	
1.000 μF		Approx. 10 nA, 100 nA, 1 μA		
10.00 μF		Approx. 100 nA, 1 μA, 10 μA		
100.0 μF	±1.9% rdg. ±5 dgt.	Approx. 1 μA, 10 μA, 100 μA	DC 2.0 V or less	
1.000 mF		Approx. 10 μA, 100 μA, 200 μA		
10.00 mF	±5.0% rdg. ±20 dgt.	Approx. 100 μA, 200 μA		

Frequency					
Range	Accuracy				
99.99 Hz					
999.9 Hz					
9.999 kHz	±0.1% rdg. +1 dgt.				
99.99 kHz (V AC Only)					

New Standard General Specifications

Drop proof	Yes
Operating temperature and humidity*1	-25°C to 65°C
Storage temperature and humidity*2	-30°C to 70°C
Applicable standards	Safety: EN61010, EMC: EN61326; Waterproof and dustproof: IP54*3

*1: 80% RH or less at up to 40°C (non-condensating), linearly decreases from 80% RH at 40°C to 25% RH or less at 65°C (non-condensating) *2: 80% RH or less (non-condensating) *3: Do not use in wet conditions.

Dimensions/Weight

87W × 185H × 47D mm (3.43"W × 7.28"H × 1.85"D), 480 g (16.9 oz.) (including batteries)

•••••••••••••••••

Safety Maximum rated voltage between CAT III 1000 V, CAT IV 600 V input terminals and ground Maximum rated voltage Between the V and COM terminals: 1000 V DC/AC between terminals Maximum rated current Between the A and COM terminals: 10 A DC/10 A AC between terminals

Accessories

TEST LEAD L9300, Instruction Manual, LR6 alkaline battery × 3

Standard DT4252 / DT4253 / DT4255 / DT4256 (Accuracy guaranteed for 1 year)

DC Voltage					
Range	Accuracy	Input Impedance			
High precision 600 mV range* ¹	±0.2% rdg. ±5 dgt.	10.2 MΩ ±1.5%			
600.0 mV	±0.5% rdg. ±5 dgt.	- 11.2 MΩ ±2.0%			
6.000 V					
60.00 V		10.3 MΩ ±2.0%			
600.0 V	±0.5% ldg. ±5 dgt.	10.2 MQ +1.5%			
1000 V		10.2 MI2 ±1.5%			

*1. DT4252 only *2. DT4252, DT4256 only. DT4252, DT4253 : ±5 dgt.

AC Voltage						
Panga	Accuracy		Input Impedance			
Range	40 Hz to 500 Hz	500 Hz or more to 1 kHz	input impedance			
6.000 V	±0.9% rdg. ±3 dgt.	±1.8% rdg. ±3 dgt.	11.2 MΩ ±2.0% // 100 pF or less			
60.00 V			10.3 MΩ ±2.0% // 100 pF or less			
600.0 V			10.2 MΩ ±1.5% // 100 pF or less			
1000 V			10.2 Mt ±1.5% // 100 pF of less			

AUTO V (Identification)			DT4253, DT4	255, DT4256 only
Panga		Accuracy		
Range	DC, 4	0 Hz to 500 Hz	500 Hz or more to 1 kHz	Input Impedance
600.0 V	0 V ±2.0% rdg. ±3 dgt.		±4.0% rdg. ±3 dgt.	900 kΩ ±20%
Crest factor 3 at up to 4000		3 at up to 4000 c	counts and reduces linearly t	o 2 at 6000 counts.
Accuracy		For AC V, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range.		
specification r	ange	With the filter ON, the accuracy is not specified at 100 Hz/500 Hz or more.		

DC A Measurement			DT4252, DT4253, DT4256 only
	Range	Accuracy	Input Impedance
٠	60.00 μA	±0.8% rdg. ±5 dgt.	1 kΩ ±5%
٠	600.0 μA	±0.8% rdg. ±5 dgt.	1 kΩ ±5%
٠	6.000 mA	±0.8% rdg. ±5 dgt.	15 Ω ±40%
•	60.00 mA	±0.8% rdg. ±5 dgt.*1	15 Ω ±40%*1
•	600.0 mA	±0.9% rdg. ±5 dgt.	35 mΩ ±30%
•	6.000 A	±0.9% rdg. ±3 dgt.*2	35 mΩ ±30%
•	10.00 A	±0.9% rdg. ±3 dgt.*2	35 mΩ ±30%

•DT4252 •DT4253 •DT4256

*1. DT4256: ±1.8% rdg. ±15 dgt. Input Impedance: 35 mΩ ±30% *2. DT4252: ±0.9% rdg. ±5 dgt.

AC A Mea	surement		DT4252, DT4256 only	
Denge	Accuracy		lanut lannadanaa	
Range	40 Hz to 500 Hz	500 Hz or more to 1 kHz	Input Impedance	
600.0 mA*1	±1.4% rdg. ±5 dgt.	±1.8% rdg. ±5 dgt.		
6.000 A	±1.4% rdg. ±3 dgt.	±1.8% rdg. ±3 dgt.	35 mΩ ±30%	
10.00 A	±1.4% lug. ±3 ugi.	±1.6% lug. ±3 ugi.		
Crest factor	3 at up to 4	000 counts and reduces li	nearly to 2 at 6000 counts	

Accuracy specification range Minimum 1% of range; add ±5 dgt. when measuring 300 counts or less. *1. DT4256 only

Electric Charge		DT4255, DT4256 only	
Range	Detection voltage range	Detection Target Frequency	
Hi	AC 40 V to AC 600 V	50 LI= / 00 LI=	
Lo	AC 80 V to AC 600 V	50 Hz / 60 Hz	

.....

During voltage detection, a continuous buzzer sounds and the red LED lights up.

Continuity Check				
Range	Accuracy Measurement Current Open-terminal Vol			Open-terminal Voltage
600.0 Ω	±0.7% rdg. ±5 dgt.		Approx. 200 µA	DC 1.8 V or less
Continuity ON threshold Approx. 25 Ω or		less (continuous buzzer	sound, red LED lights)	
Continuity OFF threshold Approx. 245 Ω or more				

Diode Check			
Range	Accuracy	Measurement Current	Open-terminal Voltage
1.500 V	±0.5% rdg. ±5 dgt.*1	Approx. 0.5 mA	DC 5.0 V or less

Buzzer sound intermittently at 0.15 V to 1.5 V, the red LED flashes. Forward threshold *1. DT4255 : ±0.5% rdg. ±8 dgt.

AC Clamp (AC Current)	DT4253, DT4255, DT4256 only		
Dongo	Accuracy		
Range	40 Hz to 1 kHz		
10.00 A			
20.00 A			
50.0 A			
100.0 A	±0.9% rdg. ±3 dgt.		
200.0 A			
500 A			
1000 A			
The optional 9010-50, 9018-50, or 9132-50 CLAMP ON PROBE is used. Accuracy does not include the error of the clamp-on probe.			
Crest factor	3 or less		
Accuracy specification range	Minimum 1% of range: add +5 dgt, when measuring at or below 5% of range		

Accuracy specification range | Minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range.

Resistance M	Resistance Measurement			
Range	Accuracy	Measurement Current	Open-terminal Voltage	
600.0 Ω	±0.7% rdg. ±5 dgt.	Approx. 200 µA		
6.000 kΩ		Approx. 100 µA		
60.00 kΩ	±0.7% rdg. ±3 dgt.*1	Approx. 10 µA	DC 1.8 V or less	
600.0 kΩ		Approx. 1 µA	DC 1.8 V or less	
6.000 MΩ	±0.9% rdg. ±3 dgt.*1	Approx. 100 nA		
60.00 MΩ	±1.5% rdg. ±3 dgt.*1 Approx. 10 nA			

Accuracy guarantee condition After zero adjustment has been performed. *1. DT4252, DT4253 : ±5 dgt.

Capacitance Measurement				
Range	Accuracy	Measurement Current	Open-terminal Voltage	
1.000 μF		Approx. 10 nA, 100 nA, 1 µA		
10.00 μF		Approx. 100 nA, 1 μA, 10 μA		
100.0 μF	±1.9% rdg. ±5 dgt.	Approx. 1 μA, 10 μA, 100 μA	DC 1.8 V or less	
1.000 mF		Approx. 10 µA, 100 µA, 200 µA]	
10.00 mF	±5.0% rdg. ±20 dgt.	Approx. 100 µA, 200 µA		

Temperature		DT4253 only	
Thermocouple Type	Range	Accuracy	
К	-40.0°C to 400.0°C (-40.0°F to 752.0°F)	±0.5% rdg. ±2°C	
K [-40.0 C t0 400.0 C (-40.0 F t0 752.0 F)] ±0.5% fdg. ±2 C			

The optional K Thermocouple DT4910 is used. Accuracy does not include the error of the K thermocouple.

Standard **General Specifications**

Durability		
Drop proof	Yes	
Operating temperature and humidity*1	-25°C to 65°C (DT4254, DT4255, DT4256) -10°C to 50°C (DT4252, DT4253)	
Storage temperature and humidity*2	-30°C to 70°C (DT4254, DT4255, DT4256) -30°C to 60°C (DT4252, DT4253)	
Applicable standards	Safety: EN61010, EMC: EN61326; Waterproof and dustproof: IP42	
*110°C to 50°C(14°F to 122°F), Up to 40°C(104°F): at 80% RH or less(non-condensating), 40°C to 45°C (104°F to 113°F): at 60% RH or less(non-condensating).		

40°C to 45°C (104°F to 113°F): at 60% RH or less(non-condensating), 45°C to 55°C (113°F to 131°F): at 50% RH or less (non-condensating) *1. Up to 40°C(104°F): at 80% RH or less(non-condensating), 40°C to 65°C (104°F to 149°F): reduces linearly 80% RH to 25% RH or less *2. 80% RH or less (non-condensating)

Dimensions/Weight

 $84W \times 174H \times 52D$ mm (3.31 $''W \times 6.85 ''H \times 2.05 ''D),$

390 g (13.8 oz.) (including batteries and holster)

Frequency		
Range	Accuracy	
99.99 Hz		
999.9 Hz		
9.999 kHz	±0.1% rdg. +1 dgt.	
99.99 kHz (V AC only)		

Safety		
Maximum rated voltage between input terminals and ground	CAT III 1000 V, CAT IV 600 V	
Maximum rated voltage between terminals	Between the V and COM terminals: DC 1000 V, AC 1000 V	
Maximum rated current between terminals	Between the A and COM terminals: DC 10 A / AC 10 A (DT4252, DT4256) Between the μA ,mAand COM terminals: DC 60 mA (DT4253 only)	
Your instrument can be used to measure voltages in excess of 1000 V DC if and only if both of		

the following conditions are satisfied: 1. The circuit under measurement is isolated from the commercial power grid. 2. The circuit under measurement is isolated from ground.

Accessories

TEST LEAD L9207-10, Instruction Manual, LR03 Alkaline battery \times 4, Holster (attached to the instrument, with a test lead holder)

DT4221 / DT4222 / DT4223 / DT4224 Pocket

(Accuracy guaranteed for 1 year)

DC Voltage		
Range	Accuracy	Input Impedance
600.0 mV		11.2 MQ +2.0%
6.000 V	0 EX units - E dist	11.2 W12 ±2.0 %
60.00 V	±0.5% rdg. ±5 dgt.	10.3 MΩ ±2.0%
600.0 V		10.2 MΩ ±1.5%

AC Voltage			
Range	Accuracy		Input Impedance
nanye	40 Hz to 500 Hz	500 Hz or more to 1 kHz	input impedance
6.000 V		±2.5% rdg. ±3 dgt.	11.2 MΩ ±2.0% // 100 pF or less
60.00 V	±1.0% rdg. ±3 dgt.	±2.0% rdg. ±3 dgt.	10.3 MΩ ±2.0% // 100 pF or less
600.0 V			10.2 MΩ $\pm 1.5\%$ // 100 pF or less
Crest factor	3 at up to 4000 counts and reduces linearly to 2 at 6000 counts.		
Accuracy	For AC V, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range		
specification range	With the filter ON, the accuracy is not specified in 100/500 Hz or more.		

AUTO V (Identification) DT42			21, DT4223 only		
Dongo	Acc	In sect land a standard			
Range	DC, 40 Hz to 500 Hz	500 Hz or more to 1 kHz	Input Impedance		
600.0 V	±2.0% rdg. ±3 dgt.	2.0% rdg. ±3 dgt. ±4.0% rdg. ±3 dgt.			
Crest factor	3 at up to 4000 counts and reduces linearly to 2 at 6000 counts.				
Accuracy	For AC V, minimum 1% of range; add ±5 dgt. when measuring at or below 5% of range.				
specification range	With the filter ON, the ad	With the filter ON, the accuracy is not specified in 100/500 Hz or more.			

Electric Charge	DT4221, DT4223 only
Detection Voltage Range	Detection Target Frequency
AC 80 V to AC 600 V	50 Hz / 60 Hz
	00112700112

During voltage detection, a continuous buzzer sounds.

Continuity Check							
Range	Accu	racy	Measurement Current	Open-terminal Voltage			
600.0 Ω	±1.0% rdg. ±5 dgt.		Approx. 200 μA	DC 1.8 V or less (DT4221, DT4222) DC 2.0 V or less (DT4223, DT4224)			
Continuity ON t	hreshold	Approx. 25 C	or less (continuous	buzzer sound)			
Continuity OFF threshold		Approx. 245	Ω or more				

Diode Check		DT4222, DT4224 only		
Range	Accuracy	Measurement Current	Open-terminal Voltage	
1.500 V	±0.9% rdg. ±5 dgt.	Approx. 0.5 mA (DT4222) Approx. 0.2 mA (DT4224)	DC 2.5 V or less	

Resistance Measurement			DT4222, DT422	3, DT4224 only
Range	Accuracy		Measurement Current	Open-terminal Voltage
600.0 Ω			Approx. 200 µA	
6.000 kΩ			Approx. 100 µA	DC 1.8 V or less
60.00 kΩ	±0.9% re	dg. ±5 dgt.	Approx. 10 µA	(DT4222)
600.0 kΩ	±1.5% rdg. ±5 dgt.		Approx. 1 µA	DC 2.0 V or less
6.000 MΩ			Approx. 100 nA	(DT4223, DT4224)
60.00 MΩ			Approx. 10 nA	
Accuracy guarantee	condition	After zero adjus	tment has been perf	ormed.

Capacitance	pacitance Measurement DT4222, DT		
Range	Accuracy	Measurement Current	Open-terminal Voltage
1.000 μF		Approx. 10 nA, 100 nA, 1 μA	
10.00 μF	1 OX and a Finite	Approx. 100 nA, 1 μA, 10 μA	DC 1.8 V or less (DT4222)
100.0 μF	±1.9% rdg. ±5 dgt.	Approx. 1 μA, 10 μA, 100 μA	()
1.000 mF		Approx. 10 μA, 100 μA, 200 μA	DC 2.0 V or less (DT4223, DT4224)
10.00 mF	±5.0% rdg. ±20 dgt.	Approx. 100 μA, 200 μA	(_ · · ·, _ · · ·,

Frequency	
Range	Accuracy
99.99 Hz	
999.9 Hz	±0.1% rdg. +2 dgt.
9.999 kHz	

Pocket General Specifications

Durability			
Drop proof	Yes		
Operating temperature and humidity*1	-10°C to 50°C (DT4221, DT4222) -10°C to 65°C (DT4223, DT4224)		
Storage temperature and humidity*2	-30°C to 60°C (DT4221, DT4222) -30°C to 70°C (DT4223, DT4224)		
Applicable standards	Safety: EN61010, EMC; EN61326, Waterproof and dustproof: IP42		
40°C to 45°C (104°F to 113°F):	p to 40°C(104°F): at 80% RH or less (non-condensating), at 60% RH or less (non-condensating), at 50% RH or less (non-condensating) ing)		

Safety Maximum rated voltage between input terminals and ground CAT III 600 V, CAT IV 300 V Maximum rated voltage between terminals Between the V and COM terminals: 600 V DC/AC

Accessories

TEST LEAD DT4911, Instruction Manual, LR03 Alkaline battery × 1, Holster (attached to the instrument, with a test lead holder)

Models

Dimensions/Weight

72W × 149H × 38D mm (2.83"W × 5.87"H × 1.50"D),

190 g (6.7 oz.) (including batteries and holster)

		High-end	d models		New stan	dard model
	Model no. (order code)	DT4281	DT4282	Model no. (order code)	DT4261	DT4261-90*
A.A.						*Z3210 set product

	Standard models				
Model no. (order code)	DT4252	DT4253	DT4255	DT4256	

HIOKI
-6000-
- Westing and
EOE
TANK COMPANY

	Pocket models				
Model no. (order code)	DT4221	DT4222	DT4223	DT4224	

Accessories/Options

L9300 / L9207-10 / DT4911 Options (accessory)

DT4261 (Bundled accessory)



TEST LEAD L9300 Cable length 95 cm (3.12 ft) Integrated cap and protective finger guard



(Bundled accessory)

DT4280/DT4250 Series

TEST LEAD L9207-10 Cable length 90 cm (2.95 ft) with one each red and black caps

with cap CAT III 1000 V, CAT IV 600 V without cap CAT II 1000 V TEST LEAD DT4911 Cable length 54 cm (1.77 ft) with one each red and black caps

DT4220 Series

(Bundled accessory)

with cap CAT IV 300 V, CAT III 600 V without cap CAT II 600 V The L4933 and L4934 can be attached to the tip of the L9300, L9207-10 and DT4911. When attaching them, make sure they are in the measuring category-II-state (with the caps removed for the L9207-10 and DT4911).





SMALL ALLIGATOR CLIP SET L4934

Option for DT4261: DC HIGH VOLTAGE PROBE P2000



DC HIGH VOLTAGE PROBE P2000

Cable length 150 cm (4.92 ft)* *Probe side CAT III 2000 V

P2000 Specifications		
Maximum input voltage	DC 2000 V (max. rated voltage between INPUT H-INPUT L)	Operat
Maximum rated voltage to earth	2000 V (Measurement Category III) anticipated transient overvoltage 15,000 V 1000 V (Measurement Category IV) anticipated transient overvoltage 12,000 V	Opera pera humi
Input resistance	$20 \text{ M}\Omega \pm 1.0\%$ (between INPUT H – INPUT L)	Storag
Output ratio	Depends on the input impedance of the connected device (example: $1/10$ when a device with an input impedance of $10 \text{ M}\Omega$ is connected)	Applic Prod perio
Overload protection	DC/AC 2200 V 1 minutes (between INPUT H – INPUTO L) DC/AC 600 V 1 minutes (between OUTPUT H – OUTPUT L)	Acce
Secondary terminal	4 mm banana terminal	

erating environment	Indoor use, pollution degree 2, altitude up to 2000 m
perating tem- erature and umidity range	Temperature: -25°C to 65°C (-13°F to 149°F) Humidity: -25°C to 40°C (-13°F to 104°F), up to 80% RH (non-condensing) 40°C to 65°C (104°F to 149°F), (the operation humidity limit falls linearly from 40°C 80% RH to 65°C 25% RH, given that there is no condensation)
orage temperature d humidity range	-30°C to 70°C (-22°F to 158°F) 90% RH or less (non-condensing)
plicable standards	Safety EN 61010
roduct warranty priod	3 years (probe body and cable part are not covered by warranty)
ccessories	L4943 connection cable*, Strap belt, Strap buckles × 2, C0205 carrying case, "Instruction Manual", "Usage Pre- cautions"
	*L4930, L4931 can be used to extend the cable



Note: Company names and product names appearing in this brochure are trademarks or registered trademarks of various companies.

HIOKI E.E. CORPORATION

C0207

Bag type for use with all field products

DISTRIBUTED BY

Test Equipment Depot - 800.517.8431 - 5 Commonwealth Ave, MA 01801 TestEquipmentDepot.com