



EL-CC-2

Single Use Temperature & Relative Humidity Monitor for the Pharmaceutical & Medical Market



- Three loggers for monitoring Ambient Pharmaceuticals, Blood and Platelets in transportation.
- Also measures 0 to 100% Relative Humidity range.
- No set-up required. One button press-to-start logging.
- Single use with up to 12+ months battery life.
- Various export options including PDF, Microsoft Excel and JPEG.

Each of the three Cold Chain loggers comes pre-configured for use in your particular application – simply press the button to start logging. During a logging session, pressing the button will light up the status LEDs to give a quick indication as to whether the temperature has exceeded an alarm condition at any point.

Once your session has been completed, tear open the IP67-rated plastic wallet to reveal the USB connector and plug it in to your PC. Use the free EasyLog CC software for Windows to download and graph the data.



GENERAL SPECIFICATIONS

Temperature	Measurement range	-30 to +70°C (-22 to +158°F)
	Internal resolution	0.1°C (0.1°F)
	Accuracy (overall error)	±0.3°C (±0.7°F) typical (see page 2)
Relative Humidity	Measurement range	0 to 100%RH (see page 2)
	Internal resolution	0.1%RH
	Accuracy (overall error)	±2%RH typical (see page 2)
IP Rating		IP67
Battery life		12 months (minimum)
Readings		32,637 temperature/ 32,637 relative humidity

INCLUDED IN THE BOX

EL-CC-2 Data Logger with integral battery

MODEL SPECIFIC

	Ambient Pharma	Blood	Platelets
High Alarm Level	25°C	10°C	24°C
Low Alarm Level	8°C	1°C	20°C
Logging Interval	10 minutes (220 days until full)		
Part Number	EL-CC-2-004 PK10	EL-CC-2-005 PK10	EL-CC-2-006 PK10

EasyLog CC Software

The simple to use software allows you to view the data graphically, in a table or export it in various formats for use in further reporting.

Once your data is in the graphing module you are able to report on time in alarm conditions as well as obtain values such as the Mean Kinetic Temperature, Minimum, Maximum and Average for both temperature and humidity.

Summary Report Serial Number: 831127464

First Reading: 18:42:02 09/05/2017 Alarm: Not Set
 Last Reading: 09:42:02 05/07/2017 Logging Rate: 5 Minutes
 Elapsed Time: 56d, 17h, 0m
 Total Readings: 16333

Conditions	Low Alarm	High Alarm	Not Set
18/05/2017	Alarm Occurrences: N/A	Alarm Occurrences: N/A	Alarm Occurrences: N/A
04/07/2017	Time in Alarm: N/A	Time in Alarm: N/A	Time in Alarm: N/A
	First Alarm Triggered: N/A	First Alarm Triggered: N/A	First Alarm Triggered: N/A
	Logged Alarm: N/A	Logged Alarm: N/A	Logged Alarm: N/A

18.7°C 16.4°C at 21:00:00
22.0°C






EL-CC-2

Single Use Temperature & Relative Humidity Monitor for the Pharmaceutical & Medical Market



YOUR EL-CC-2


- 1 Start / Status button
- 2 Status LEDs
- 3 USB connector
- 4 Tear to open
- 5 Mounting point
- 6 Model type

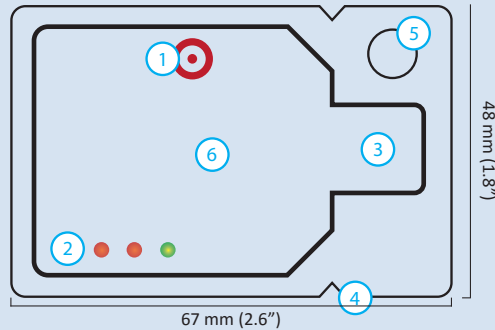


This unit can be quickly customised for use in multiple markets. If you have a specific monitoring application, call us today.

SENSOR ACCURACY & INFORMATION


Typical and maximal tolerance for temperature sensor in °C.

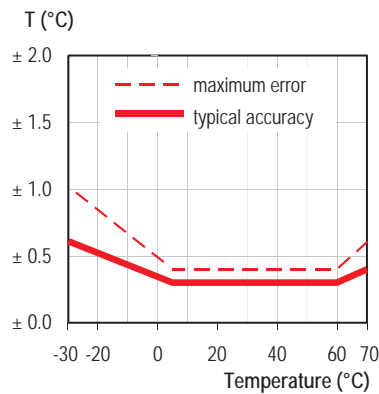


Typical and maximal tolerance at 25°C for relative humidity.

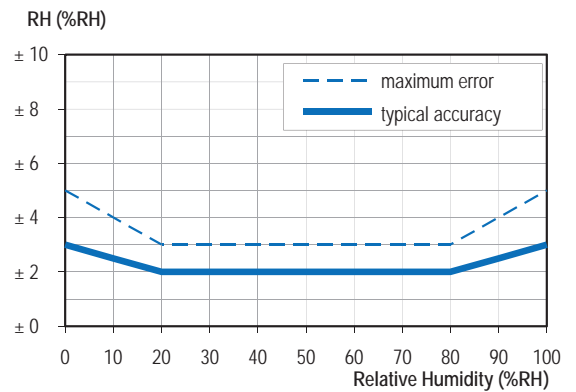

Typical accuracy of relative humidity measurements given in %RH for temperatures 0 to 80°C.

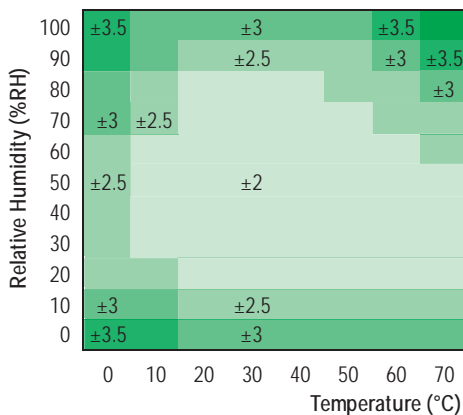

Operating conditions

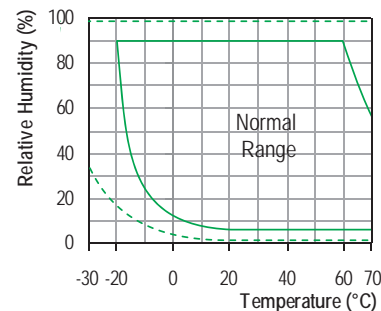

Long term exposure to humidity levels outside of the 'normal' range may temporarily offset RH measurements (±3%RH after 60 hours). Once returned to less extreme conditions the device will slowly return towards calibration state.

When tracking changes in ambient conditions, the response time of the humidity sensor in your data logger is approximately 20 minutes to reach 90% of the reading. However, if you are measuring step changes in humidity it is advised that you leave the unit for up to four hours to ensure that it has enough time to settle at the new level.

It is worth remembering that the value of relative humidity is of course sensitive to temperature variation. As an example, at a relative humidity of ~90%RH at ambient temperature, a variation in temperature of 1°C will result in a change of up to -5%RH. Therefore when comparing multiple devices or calibrating them, any temperature variations must be considered.



99 Washington Street
Melrose, MA 02176
Phone 781-665-1400
Toll Free 1-800-517-8431



Visit us at www.TestEquipmentDepot.com