

150 & 450 Series Waterproof Handheld Meter

pH/mV Operation Instructions

EUTECH
INSTRUMENTS
Technology Made Easy ...

OAKTON[®]

Models:



pH 150
pH/mV


pH 450
pH/mV/ISE

PC 450
pH/mV/Con

PD 450
pH/mV/DO

Getting Started/Connections

After installing (2) AA batteries and/or connecting the optional 110/220 VAC power supply, connect the desired sensors to the corresponding ports.

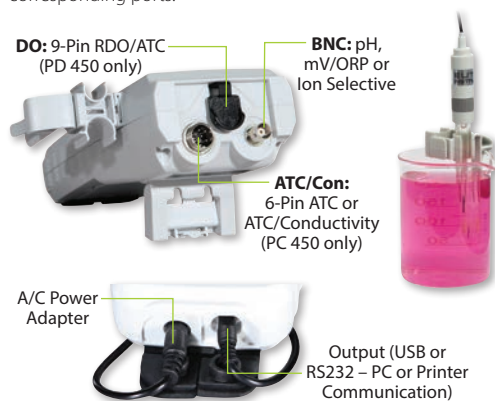

12 mm and 16 mm probes can utilize the **Grip-Clip™** to attach one or more sensors to a beaker and to the instrument as needed. The stand can be extended as shown above or used for wall-mounting.

Keypad Functions

	Press once to power ON in the mode that was previously used. Press again to turn backlight on for one minute or off (450 series only). Hold for 3 seconds to power OFF.
	Toggle between measurement and calibration modes. In SETUP mode, BACK serves to return to the previous menu option or setting.
	Confirm calibration values in CAL mode. Confirm selections in SETUP mode. Freeze or release the measured reading.
	Customize instrument settings and preferences. (See also Setup Programs)
	Toggle between available measurement types.
	Save measurement into memory. Increase value or scroll up in SETUP or manual calibration.
	Recall saved values from memory. Decrease value or scroll down in SETUP or manual calibration.
	Send output data to printer or computer. (450 series only).

Setup Programs

To access the settings below, press **SETUP**. Up/down arrows will display the available options. Press **ENTER** to accept the desired setting, or **BACK** to return to the previous option and/or exit.

Configuration Options

- Ready indicator **ON / OFF /** or Automatic **HOLD** when stable
- Choose °Celsius or °Fahrenheit

pH Buffer Options

- Select the desired pH Buffer Calibration Group:
 - USA** (1.68, 4.01, 7.00, 10.01, 12.45) or
 - NIST** (1.68, 4.01, 6.86, 9.18, 12.45) or
 - DIN** (1.09, 3.06, 4.65, 6.79, 9.23, 12.75) or
 - MAN** (manual adjustment of any custom pH values that are ≥ 1 pH unit apart. 450 series only)
- Select number of calibration points

Select Calibration Due Reminder

- Set number of days from **0-60** for desired parameter

View Calibration Data

- Press **ENTER** to view each point that is calibrated.

View Electrode Data

- Press **ENTER** to view **mV Offset** and **Slope %** of the measured reading.

System Settings

- Data Logging:
 - MANUAL** upon key press only
 - TIMED** interval. Choose (**SEC / MIN / HOUR**) interval.
- Automatic shut off after 10 minutes. Choose **ON** or **OFF**.
- Clock Settings:
 - Date: Choose **USA** (MM/DD/YYYY) or **Euro** (DD/MM/YYYY).
 - Time: Choose (**24HR** or **12HR**). If 12HR, choose **AM** or **PM**.
- Set Printer Type:
 - CSV** (Comma Separated Values) – best format for computer
 - Printer** (Text) – best format for printer.
- Choose Manual (**MAN**) upon key press or **TIMED** interval. If timed, choose (**SEC / MIN / HOUR**).

Reset

- **NO**. Exits from reset menu options without action.
- **FACTORY RESET**. Returns all settings except date/time and ATC calibration to factory default values after **ENTER** is pressed then restarts meter.
- **DATA RESET**. Erases data stored in memory while retaining other settings after **ENTER** is pressed.
- **CALIBRATION RESET**. Erases non-ATC calibration data while retaining other settings after **ENTER** is pressed.

pH Calibration

For best results, periodic calibration with known, accurate standards is recommended. Calibrate with standards that bracket your intended measuring range while including a neutral standard (pH 7.00 or 6.86). For example, if you expect to measure samples from pH 6.2 to pH 9.5, calibration with 4.01, 7.00, and 10.01 standards will work well. Provide stirring for best results. After calibration with two or more points, the active slope segment of the measurement will be visible on the bottom display during measurement. 100 % slope will be shown if only one calibration point is performed and "- - -" if no calibration is performed. The meter will automatically return to measurement mode upon successful completion of the number of specified calibration points. To specify a different number of pH calibration points, see **pH Buffer Options**.

Using Automatic Buffer Recognition

1. While in pH measurement mode, dip the pH and ATC sensor(s) into your first standard, then press **CAL**. The primary display will search for the nearest standard value, while the secondary display will show the un-adjusted value.
2. When the **"READY"** indicator appears, press **ENTER** to accept. The primary reading will flash **"DONE"**.
3. Rinse your electrode(s) then dip into the next pH standard. The primary display will search for the nearest standard value that has not yet been calibrated, while the secondary display will show the unadjusted value. When the **"READY"** indicator appears, press **ENTER** to accept.
4. To calibrate another pH standard repeat Step 3 or press **MEAS** to return to pH measurement mode.

Using Manual Recognition / Custom Buffers (450 Series Only)

1. While in pH measurement mode, dip the pH and ATC sensor(s) into your first standard then press **CAL**.
2. When the **READY** indicator appears, use up/down arrows to adjust the primary reading to match the standard value at the measured temperature, then press **ENTER**.
3. Rinse your electrode(s) then repeat Step 2 with a standard that is ≥ 1 pH unit from the previous standard value.
4. To calibrate another pH standard, repeat Step 3 or press **MEAS** to return to pH measurement mode.

mV Offset Adjustment

1. While in mV measurement mode, dip the ORP and ATC sensors into a solution with a known mV value (i.e. Zobel, Light's, quinhydrone, or iodide/triiodide) and stir.
2. When the **"READY"** indicator appears, use up/down arrows to adjust the primary reading to match the mV value at the measured temperature, then press **ENTER**. The meter allows an adjustable maximum value of ± 200 mV from the factory default mV value. When an offset has been stored successfully, R.mV replaces mV.

Temperature Calibration/Manual ATC

1. Press **CAL** from any measurement, then press **MODE**.
2. Skip to step 3 for manual ATC, otherwise, dip the temperature sensor into a solution with a known accurate temperature. The upper display shows the active temperature while the lower display shows the factory default temperature without adjustment.
3. Use up/down arrows to adjust the upper display. Press **ENTER** to accept the calibration temperature. The maximum adjustable value is ± 10 °C (or ± 18 °F) from factory default.

Error Messages

- ERR** "ERR" will appear when an error condition exists or the incorrect key is pressed. Common examples include:
- Pressing **ENTER** during calibration before the **"READY"** indicator appears. Wait for the **"READY"** indicator before pressing **ENTER**.
 - **UR** (Under Range) • **OR** (Over Range)

Intended Use, Maintenance & Precautions

These handheld meters use sensors to detect various parameters for water-based measurements. For routine maintenance disconnect the power cord or battery, then dust or wipe the display using a damp cloth. If necessary, warm water or a mild water based detergent can be used. Immediately remove any spilled substance from contact with the meter using the proper cleaning procedure for the type of spill.

- Do not use this equipment in potentially explosive atmospheres.
- Refer to the electrode instructions for use, storage and cleaning.
- Ensure that no liquid enters the instrument.
- Do not use any aggressive cleaning chemicals (solvents or similar agents).
- There are no user serviceable parts inside. Attempts to service internal parts may void the warranty.
- **WARNING:** No modification of this equipment is allowed.

Instrument Operating Conditions

Operating Ambient Temp.	5 to 45 °C
Operating Relative Humidity	5 to 85 % non-condensing
Storage Temp.	-20 to +60 °C
Storage Relative Humidity	5 to 85 % non-condensing
Pollution	Degree 2
Overvoltage	Category II
Weight	500 g
Size (L x W x H)	21.15 x 9.87 x 5.85 cm
Regulatory & Safety	CE, TUV 3-1, FCC Class A
Power Rating	DC Input: 9 VDC 1 A 2 x AA (LR6) 1.5 V batteries (replace batteries when battery sign blinks)
Battery Requirement	
Vibration	Shipping/handling per ISTA #1A
Shock	Drop test in packaging per ISTA #1A
Enclosure (Designed To Meet)	IP67 (using rubber covers)
Universal Power Adapter Operating Conditions	
Operating Ambient Temp.	0 to 50 °C
Operating Relative Humidity	0 to 90 % non-condensing
Storage Temp.	-20 to +75 °C
Storage Relative Humidity	0 to 90 % non-condensing
Pollution	Degree 2
Overvoltage	Category II
Power Rating	I/P: 100 - 240 V, 50/60 Hz, 0.3A O/P: 9 VDC 1 A

Test Equipment Depot
1-800-517-8431

99 Washington Street
Melrose, MA 02176
Phone 781-665-1400
Toll Free 1-800-517-8431

Visit us at www.TestEquipmentDepot.com