

Continental Control Systems (CCS) ACT Series Split-Core Current Transformer (CT) Connection Instructions

For use with HOBOb® H22, U30, and RX3000 Series Data Loggers

Applies to these CCS ACT Series CTs

Onset Part No.	Rated Current	Output	CCS Part No.
T-ACT-0750-020	20 Amps	0-333mV AC representing 0 to 20 Amps AC	ACTL-0750-020
T-ACT-0750-050	50 Amps	0-333mV AC representing 0 to 50 Amps AC	ACTL-0750-050
T-ACT-0750-100	100 Amps	0-333mV AC representing 0 to 100 Amps AC	ACTL-0750-100
T-ACT-0750-250	250 Amps	0-333mV AC representing 0 to 250 Amps AC	ACTL-0750-250



DANGER!—HIGH VOLTAGE HAZARD



Installing CTs in an energized electrical enclosure or on any energized conductor can result in severe injury or death. These CTs are for installation by qualified personnel only. To avoid electrical shock, do not perform any installation or servicing of these CTs unless you are qualified to do so. Disconnect and lock-out all power sources during installation and servicing.

This document provides instructions on connecting the CCS ACT series CTs listed above to the FlexSmart™ TRMS Module used with HOBOb H22, U30, or RX3000 series data loggers. It also lists configuration values used by HOBObware® software to configure the logger for each CT.

Required


- Selected CCS ACT series CT
- HOBOb H22, U30, and RX3000 Series Data Logger
- FlexSmart TRMS Module, Onset Part No: S-FS-TRMSA (for H22 series only) or S-FS-TRMSA-D (for H22, U30, and RX3000 series)
- HOBObware software, version 3.5 or higher (for H22 and U30 series)
- HOBOblink (for RX3000 series)



CCS Accu-CT
Split-Core Current Transformer


Dimensions

- Width: 60.4 mm (2.38 in.)
- Height: 61.0 mm (2.40 in.)
- Thickness: 22.9 mm (0.90 in.)
- Window: 20.0 mm (0.78 in.)
- Weight: 172 grams (6.1 oz)

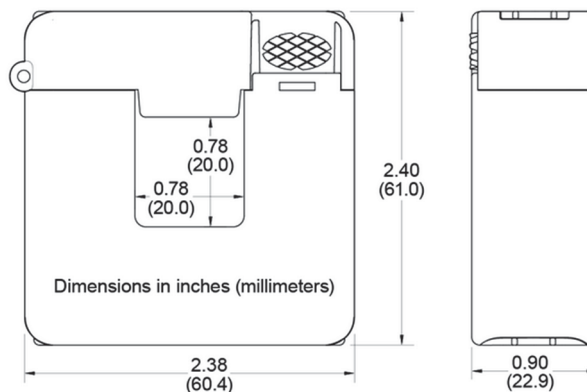

Continental Control Systems (CCS) ACT Series CT Connection Instructions

Connecting the CT to the FlexSmart TRMS Module

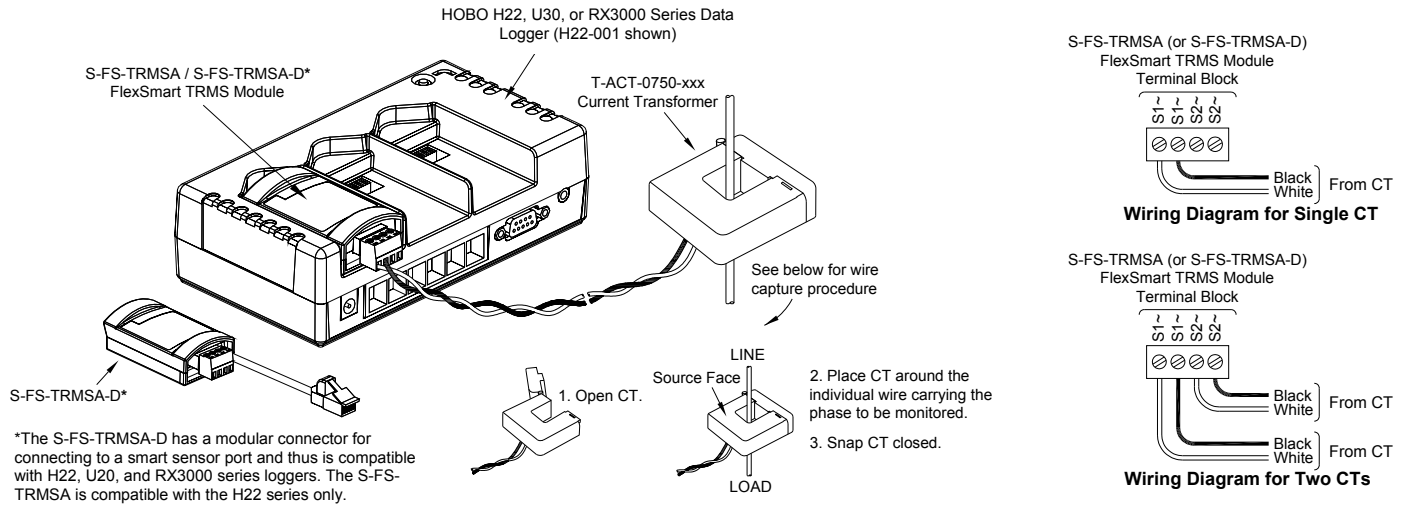

Configuring the Data Logger for the CT using HOBOWare Software

HOBOWare software provides configuration files for the CTs. The table below lists the recommended configuration values for each CT that these files contain. For information on loading configuration files, refer to the software documentation.

Onset Part No:	Channel Name	Raw Value 1 (mV)	Raw Value 2 (mV)	Scaled Value 1	Scaled Value 2	Scaled Units
T-ACT-0750-020	Current	0	333.33	0	20	A
T-ACT-0750-050	Current	0	333.33	0	50	A
T-ACT-0750-100	Current	0	333.33	0	100	A
T-ACT-0750-250	Current	0	333.33	0	250	A